

**SARS-CoV-2 Assay (Panther Fusion® System)**

For Emergency Use Authorization (EUA) only

For *in vitro* diagnostic use only

Rx only

**CONTENTS**

**General Information** .....2  
    Intended Use .....2  
    Summary and Explanation of the Test .....3  
    Principles of the Procedure .....3  
    Warnings and Precautions .....4  
    Reagent Storage and Handling Requirements .....7  
    Specimen Collection and Storage .....8  
    Specimen Pooling - Determining Appropriate Strategy for Implementation and Monitoring .9  
    Preparing Samples for Pooling .....9  
    Specimen Transport .....12  
**Panther Fusion System** .....13  
    Reagents and Materials Provided for the Panther Fusion SARS-CoV-2 Assay .....13  
    Materials Required and Available Separately .....14  
    Panther Fusion System Test Procedure .....15  
    Procedural Notes .....17  
**Quality Control** .....18  
**Interpretation of Results** .....19  
**Limitations** .....20  
**Conditions of Authorization for Labs** .....21  
**Panther Fusion SARS-CoV-2 Assay Performance** .....23  
    Analytical Sensitivity .....23  
    Inclusivity .....23  
    Analytical Specificity and Microbial Interference .....24  
    Clinical Performance .....25  
**Bibliography** .....31  
**Appendix A: Specimen Pooling Implementation and Monitoring Guidelines** .....32

## General Information

### Intended Use

The Panther Fusion® SARS-CoV-2 assay is a real-time RT-PCR *in vitro* diagnostic test intended for the qualitative detection of RNA from SARS-CoV-2 isolated and purified from nasopharyngeal (NP) and oropharyngeal (OP) swab specimens, nasopharyngeal washes/aspirates or nasal aspirates, and bronchoalveolar lavage specimens (collected by a healthcare provider) and anterior nasal (nasal) and mid-turbinate nasal swab specimens (collected under observation of or by a healthcare provider) from individuals who meet COVID-19 clinical and/or epidemiological criteria, as well as NP and OP swab specimens (collected by a healthcare provider) and nasal and mid-turbinate nasal swab specimens (collected under observation of or by a healthcare provider) from any individual, including from individuals without symptoms or other reasons to suspect COVID-19. The Panther Fusion SARS-CoV-2 assay is for use only under Emergency Use Authorization (EUA) in laboratories certified under the Clinical Laboratory Improvement Amendments of 1988 (CLIA), 42 U.S.C.§263a, that meet requirements to perform high complexity tests.

This test is also for the qualitative detection of nucleic acid from SARS-CoV-2 in pooled samples containing up to 5 individual NP or OP swabs (collected by a healthcare provider), nasal, or mid-turbinate nasal swabs (collected under observation of or by a healthcare provider), where each specimen is collected using individual vials containing transport media. Negative results from pooled testing should not be treated as definitive. If a patient's clinical signs and symptoms are inconsistent with a negative result or if results are necessary for patient management, then the patient should be considered for individual testing. Specimens included in pools with a positive or invalid result must be tested individually prior to reporting a result. Specimens with low viral loads may not be detected in sample pools due to the decreased sensitivity of pooled testing. For specific patients, whose specimen(s) were the subject of pooling, a notice that pooling was used during testing must be included when reporting the result to the clinician or healthcare provider.

Results are for the identification of SARS-CoV-2 RNA. The SARS-CoV-2 RNA is generally detectable in upper and lower respiratory specimens during the acute phase of infection. Positive results are indicative of the presence of SARS-CoV-2 RNA, clinical correlation with patient history and other diagnostic information is necessary to determine patient infection status. Positive results do not rule out bacterial infection or co-infection with other viruses. The agent detected may not be the definite cause of disease. Laboratories within the United States and its territories are required to report all results to the appropriate public health authorities.

Negative results do not preclude SARS-CoV-2 infection and should not be used as the sole basis for patient management decisions. Negative results must be combined with other clinical observations, patient history, and epidemiological information.

The Panther Fusion SARS-CoV-2 assay on the Panther Fusion system is intended for use by qualified clinical laboratory personnel specifically instructed and trained in the operation of the Panther Fusion system and *in vitro* diagnostic procedures. The Panther Fusion SARS-CoV-2 assay is only for use under the Food and Drug Administration's Emergency Use Authorization.

## Summary and Explanation of the Test

Coronaviruses are a large family of viruses which may cause illness in animals or humans. In humans, several coronaviruses are known to cause respiratory infections ranging from the common cold to more severe diseases such as Middle East Respiratory Syndrome (MERS) and Severe Acute Respiratory Syndrome (SARS). The most recently discovered coronavirus, SARS-CoV-2, causes the associated coronavirus disease COVID-19. This new virus and disease were unknown before the outbreak began in Wuhan, China, in December 2019.<sup>1</sup>

The most common symptoms of COVID-19 are fever, tiredness, and dry cough. Some patients may have aches and pains, nasal congestion, runny nose, sore throat, new loss of taste or smell, or diarrhea. These symptoms are usually mild and begin gradually. Some people become infected but don't develop any symptoms and don't feel unwell. The disease can spread through respiratory droplets produced when an infected person coughs or sneezes. These droplets can land in the mouths or noses of people who are nearby or possibly be inhaled into the lungs.<sup>2</sup> These droplets also can land on objects and surfaces around the person.<sup>3</sup> Other people may acquire SARS-CoV-2 by touching these objects or surfaces, then touching their eyes, nose, or mouth.

The virus that causes COVID-19 is infecting people and spreading easily from person to person. On March 11, 2020, the COVID-19 outbreak was characterized as a pandemic by the World Health Organization (WHO).<sup>4,5</sup>

## Principles of the Procedure

The Panther Fusion SARS-CoV-2 assay involves the following steps: sample lysis, nucleic acid capture, elution transfer, and multiplex RT-PCR when analytes are simultaneously amplified and detected. Nucleic acid capture and elution takes place in a single tube on the Panther Fusion system. The eluate is transferred to the Panther Fusion system reaction tube containing the assay reagents. Multiplex RT-PCR is then performed for the eluted nucleic acid on the Panther Fusion system.

**Nucleic acid capture and elution:** Prior to processing and testing on the Panther Fusion system, specimens need to be transferred to a Specimen Lysis Tube containing specimen transport media (STM) that lyses the cells, releases target nucleic acid and protects them from degradation during storage.

The Internal Control-S (IC-S) is added to each test specimen and controls via the working Panther Fusion Capture Reagent-S (wFCR-S). The IC-S in the reagent monitors specimen processing, amplification and detection.

Capture oligonucleotides hybridize to nucleic acid in the test specimen. Hybridized nucleic acid is then separated from the specimen in a magnetic field.

Wash steps remove extraneous components from the reaction tube. The elution step elutes purified nucleic acid. During the nucleic acid capture and elution step, total nucleic acid is isolated from specimens.

**Elution transfer and RT-PCR:** During the elution transfer step, eluted nucleic acid is transferred to a Panther Fusion reaction tube already containing oil and reconstituted mastermix.

Target amplification occurs via RT-PCR. A reverse transcriptase generates a DNA copy of the target sequences. Target specific forward and reverse primers and probes then amplify targets

while simultaneously detecting and discriminating multiple target types via multiplex RT-PCR. To safeguard against potential mutational drift in the SARS-CoV-2 genome, the Panther Fusion SARS-CoV-2 assay amplifies and detects two conserved regions of the ORF1ab gene in the same fluorescence channel. The two regions are not differentiated and amplification of either or both regions leads to a fluorescence signal.

The Panther Fusion system compares the fluorescence signal to a predetermined cut-off to produce a qualitative result for the presence or absence of the analyte.

The analytes and the channel used for their detection on the Panther/Panther Fusion system are summarized in the table below.

Analyte	Gene Targeted	Instrument Channel
SARS-CoV-2	ORF1ab Region 1 ORF1ab Region 2	ROX
Internal Control	Not applicable	RED677

## Warnings and Precautions

- A. For *in vitro* diagnostic use. For use under an Emergency Use Authorization (EUA) only.
- B. This product has not been FDA cleared or approved but has been authorized for emergency use by FDA under an EUA for use by authorized laboratories.
- C. This product has been authorized only for the detection of nucleic acid from SARS-CoV-2, not for any other viruses or pathogens.
- D. The emergency use of this product is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of *in vitro* diagnostics for detection and/or diagnosis of COVID-19 under Section 564(b)(1) of the Federal Food, Drug, and Cosmetic Act, 21 U.S.C. §360bbb-3(b)(1), unless the declaration is terminated or authorization is revoked sooner.
- E. Carefully read this entire package insert and the *Panther/Panther Fusion System Operator's Manual*.
- F. The Panther Fusion Enhancer Reagent-S (FER-S) is corrosive, harmful if swallowed and causes severe skin burns and eye damage.
- G. Only personnel adequately trained on the use of this assay and in handling potentially infectious materials should perform these procedures. If a spill occurs, immediately disinfect using appropriate site procedures.
- H. Handle all specimens as if infectious using safe laboratory procedures. Refer to Interim Laboratory Biosafety Guidelines for Handling and Processing Specimens Associated with 2019-nCoV. <https://www.cdc.gov/coronavirus/2019-ncov/lab/lab-biosafety-guidelines.html>.
- I. Specimens may be infectious. Use Universal Precautions when performing this assay. Proper handling and disposal methods should be established by the laboratory director. Only personnel adequately trained in handling infectious materials should be permitted to perform this diagnostic procedure.<sup>6</sup>

- J. If infection with 2019-nCoV is suspected based on current clinical screening criteria recommended by public health authorities, specimens should be collected with appropriate infection control precautions.
- K. Use only supplied or specified disposable laboratory ware.
- L. Use appropriate personal protective equipment when collecting and handling specimens from individuals suspected of being infected with SARS-CoV-2 as outlined in CDC Interim Laboratory Biosafety Guidelines for Handling and Processing Specimens Associated with 2019 Novel Coronavirus (2019-nCoV).
- M. Wear disposable, powderless gloves, protective eye wear, and laboratory coats when handling specimens and reagents. Wash hands thoroughly after handling specimens and reagents.
- N. Dispose of all material that has come into contact with specimens and reagents in accordance with applicable national, international, and regional regulations.
- O. Expiration dates listed on the Panther Fusion Specimen Lysis Tubes pertain to the transfer of sample into the tube and not to testing of the sample. Specimens collected/transferred any time prior to these expiration dates are valid for testing provided they are transported and stored in accordance with the appropriate package insert, even if these expiration dates have passed.
- P. Maintain proper storage conditions during specimen shipping to ensure the integrity of the specimen. Specimen stability under shipping conditions other than those recommended has not been evaluated.
- Q. Avoid cross-contamination during the specimen handling steps. Specimens can contain extremely high levels of virus or other organisms. Ensure that specimen containers do not come in contact with one another, and discard used materials without passing them over any open containers. Change gloves if they come in contact with specimens.
- R. Do not use the reagents and controls after the expiration date.
- S. Store assay components at the recommended storage condition. See *Reagent Storage and Handling Requirements* (page 7), and *Panther Fusion System Test Procedure* (page 15) for more information.
- T. Do not combine any assay reagents or fluids. Do not top off reagents or fluids; the Panther Fusion system verifies reagent levels.
- U. Avoid microbial and ribonuclease contamination of reagents.
- V. Quality control requirements must be performed in conformance with local, state, and/or federal regulations or accreditation requirements and your laboratory's standard quality control procedures.
- W. Do not use the assay cartridge if the storage pouch has lost its seal or if the assay cartridge foil is not intact. Contact Hologic if either occurs.
- X. Do not use the fluid packs if the foil seal is leaking. Contact Hologic if this occurs.

- Y. Handle the assay cartridges with care. Do not drop or invert assay cartridges. Avoid prolonged exposure to ambient light.
- Z. Do not use material that may contain Guanidinium thiocyanate or any guanidine-containing materials on the instrument. Highly reactive and/or toxic compounds may form if combined with sodium hypochlorite.
- AA. Some reagents in this kit are labeled with risk and safety symbols.
- AB. Contamination may occur if carryover of samples is not adequately controlled during sample pool preparation, handling, and processing.
- AC. Testing of pooled specimens may impact the detection capability of the Panther Fusion SARS-CoV-2 assay and impact sensitivity.

**Note:** For information on any hazard and precautionary statements that may be associated with reagents, refer to the Safety Data Sheet Library at [www.hologicds.com](http://www.hologicds.com).

	<p><b>Panther Fusion Oil / Aptima Oil</b>  <i>Polydimethylsiloxane 95-100%</i></p>
	<p><b>WARNING</b>            H315 - Causes skin irritation            H319 - Causes serious eye irritation            P264 - Wash face, hands and any exposed skin thoroughly after handling            P280 - Wear protective gloves/protective clothing/eye protection/face protection            P305 + P351 + P338 - IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses if present and easy to do. Continue rinsing            P337 + P313 - If eye irritation persists: Get medical advice/attention            P302 + P352 - IF ON SKIN: Wash with plenty of soap and water            P332 + P313 - If skin irritation occurs: Get medical advice/attention            P362 - Take off contaminated clothing and wash before reuse</p>
	<p><b>Panther Fusion Enhancer Reagent-S</b>  <i>Lithium Hydroxide, Monohydrate 5-10%</i></p>
	<p><b>DANGER</b>            H302 - Harmful if swallowed            H314 - Causes severe skin burns and eye damage            P260 - Do not breathe dust/fume/gas/mist/vapors/spray            P264 - Wash face, hands and any exposed skin thoroughly after handling            P270 - Do not eat, drink or smoke when using this product            P280 - Wear protective gloves/protective clothing/eye protection/face protection            P301 + P312 - IF SWALLOWED: Call a POISON CENTER or doctor/physician if you feel unwell            P301 + P330 + P331 - IF SWALLOWED: rinse mouth. Do NOT induce vomiting            P303 + P361 + P353 - IF ON SKIN (or hair): Remove/Take off immediately all contaminated clothing. Rinse skin with water/shower            P304 + P340 - IF INHALED: Remove victim to fresh air and keep at rest in a position comfortable for breathing            P305 + P351 + P338 - IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing            P310 - Immediately call a POISON CENTER or doctor/physician            P330 - Rinse mouth            P363 - Wash contaminated clothing before reuse</p>

## Reagent Storage and Handling Requirements

A. The following table provides storage and handling requirements for this assay.

Reagent	Unopened Storage	On Board/ Open Stability <sup>1</sup>	Opened Storage
Panther Fusion Open Access RNA/DNA Enzyme Cartridge	2°C to 8°C	60 days	2°C to 8°C
Panther Fusion Capture Reagent-S (FCR-S)	15°C to 30°C	30 days	15°C to 30°C
Panther Fusion SARS-CoV-2 Assay PPR Solution	-15°C to -85°C	3 days	On-board instrument
Panther Fusion Enhancer Reagent-S (FER-S)	15°C to 30°C	30 days	15°C to 30°C
Panther Fusion Internal Control-S (IC-S)	2°C to 8°C	(In wFCR-S)	Not applicable
Panther Fusion Elution Buffer	15°C to 30°C	60 days	15°C to 30°C
Panther Fusion Oil	15°C to 30°C	60 days	15°C to 30°C
Panther Fusion SARS-CoV-2 Positive Control	2°C to 8°C	Single use vial	Not applicable-single use
Panther Fusion SARS-CoV-2 Negative Control	2°C to 8°C	Single use vial	Not applicable-single use

When reagents are removed from the Panther Fusion system, return them immediately to their appropriate storage temperatures.

<sup>1</sup> On board stability starts at the time the reagent is placed on the Panther Fusion system for the Panther Fusion Open Access RNA/DNA Enzyme cartridge, SARS-CoV-2 Assay PPR Solution, FCR-S, FER-S, and IC-S. On board stability starts for the Panther Fusion Reconstitution Buffer I, Panther Fusion Elution Buffer and Panther Fusion Oil when the reagent pack is first used.

- B. Working Panther Fusion Capture Reagent-S and Panther Fusion Enhancer Reagent-S are stable for 60 days when capped and stored at 15°C to 30°C. Do not refrigerate.
- C. Discard any unused reagents that have surpassed their on board stability.
- D. Controls are stable until the date indicated on the vials.
- E. Avoid cross-contamination during reagent handling and storage.
- F. **Do not freeze reagents. Once thawed, do not re-freeze the Panther Fusion SARS-CoV-2 assay PPR Solution.**

## Specimen Collection and Storage

**Specimens** - Clinical material collected from patient placed in an appropriate transport system. For the Panther Fusion SARS-CoV-2 assay, this includes NP, nasal and OP swab specimens in viral transport medium (VTM/UTM), saline, Liquid Amies, or specimen transport medium (STM) and LRT specimens.

**Samples** - Represents a more generic term to describe any material for testing on the Panther Fusion System including specimens, specimens transferred into a Panther Fusion Specimen Lysis Tube and controls.

**Note:** *Handle all specimens as if they contain potentially infectious agents. Use Universal Precautions.*

**Note:** *Take care to avoid cross-contamination during specimen handling steps. For example, discard used material without passing over open tubes.*

### A. Swab specimen collection

Collect NP swab, nasal swab, and OP swab specimens according to standard technique using a polyester-, rayon-, or nylon-tipped swab. Immediately place the swab specimen into 3 mL of VTM or UTM. Swab specimens may alternatively be added to saline, Liquid Amies or STM. The Aptima Multitest Swab Specimen Collection Kit may be used for the collection of OP and nasal swab samples.

The following types of VTM/UTM were verified for use.

- Remel MicroTest M4, M4RT, M5 or M6 formulations
- Copan Universal Transport Medium
- BD Universal Viral Transport Medium

**Note:** *Do not use medium that may contain Guanidium thiocyanate or any guanidinecontaining material.*

### B. Nasopharyngeal Wash/aspirate and Nasal Aspirate Specimen Collection

Collect nasopharyngeal wash/aspirate and nasal aspirate specimens according to standard techniques.

### C. LRT specimen collection

Collect bronchoalveolar lavage fluid and bronchial wash specimens according to standard techniques.

### D. Specimen processing using the Panther Fusion Specimen Lysis Tube

1. Prior to testing on the Panther Fusion system, transfer swab or LRT specimen\* to a Panther Fusion Specimen Lysis Tube.
  - For swab specimens, transfer 500 µL of the collected specimen to a Panther Fusion Specimen Lysis Tube. Affix the provided penetrable cap.
  - For LRT specimens, transfer 250 uL of the LRT specimen (avoid transferring mucus) and 250 uL of VTM/UTM to a Panther Fusion Specimen Lysis Tube. Affix the provided penetrable cap.

**\*Note:** *When testing frozen specimen, allow specimen to reach room temperature prior to processing.*



2. Storing specimens before testing
  - a. After collection, specimens can be stored at 2°C to 8°C up to 96 hours before transferred to the Panther Fusion Specimen Lysis Tube. Remaining specimen volumes can be stored at ≤-70°C.
  - b. Specimens in the Panther Fusion Specimen Lysis Tube may be stored under one of the following conditions:
    - 15°C to 30°C up to 6 days or
    - 2°C to 8°C up to 3 months.

**Note:** *It is recommended that specimens transferred to the Panther Fusion Specimen Lysis Tube are stored capped and upright in a rack.*

- E. Samples on board the Panther Fusion system may be archived for additional testing at a later time.
- F. Storing samples after testing
  1. Samples that have been assayed should be stored upright in the rack under one of the following conditions:
    - 15°C to 30°C up to 6 days or
    - 2°C to 8°C up to 3 months.
  2. The samples should be covered with a new, clean plastic film or foil barrier.
  3. If assayed samples need to be frozen or shipped, remove the penetrable cap and place a new non-penetrable cap on the specimen tubes. If samples need to be shipped for testing at another facility, recommended temperatures must be maintained. Prior to uncapping previously tested and recapped samples, specimen transport tubes must be centrifuged for 5 minutes at 420 Relative Centrifugal Force (RCF) to bring all of the liquid down to the bottom of the tube. Avoid splashing and cross-contamination.

## Specimen Pooling - Determining Appropriate Strategy for Implementation and Monitoring

When considering specimen pooling, laboratories should evaluate the appropriateness of a pooling strategy based on the positivity rate in the testing population and the efficiency of the pooling workflow. Refer to Appendix A of these instructions for Use for additional information **prior** to implementation of specimen pooling.

## Preparing Samples for Pooling

The following upper respiratory tract specimens authorized under the Emergency Use Authorization of the Panther Fusion SARS-CoV-2 assay may be tested with sample pooling. This includes nasopharyngeal, oropharyngeal, mid-turbinate and nasal swab specimens collected into VTM/UTM, saline, Liquid Amies and Specimen Transport Media (STM) Only specimens collected into a single type of media may be combined for each sample pool. For example, specimens collected in VTM/UTM should not be combined into a pool with specimens collected in Liquid Amies. Additionally, both neat specimens (those not prepared with STM for testing) and specimens prepared with STM for testing may be included in sample pooling. Each sample pool must be comprised of only neat or only STM prepared specimens. Recommended sample pooling workflow options for different specimen types are provided.

**For Specimens Collected in VTM/UTM, Saline, Liquid Amies**

Customers may choose from one of the following two options to perform specimen processing for pooled samples using Specimen Lysis Tubes with the Panther Fusion SARS-CoV-2 assay.

**Note:** Hologic testing was performed using pooled samples generated from samples collected in a single collection medium type (i.e., VTM/UTM). Combination of multiple transport media types (e.g., VTM/UTM, saline, and Liquid Amies) in a single pool has not been evaluated.

**Option 1:****Specimen Preparation Instructions for Neat Samples Pooled Directly into a Panther Fusion Specimen Lysis Tube (Panther Fusion SLT)**

Perform the following procedure when pooling specimens collected in VTM/UTM, saline, or Liquid Amies by transferring samples directly into a Panther Fusion Specimen Lysis Tube (Panther Fusion SLT).

- A. Determine the appropriate volume required from each individual specimen based on the pool size being implemented. The required specimen to STM ratio in the assay test sample must be maintained for sample pooling. For example, if a pool size of 5 specimens is being utilized, 100 µL of each individual specimen (500 µL total) is required.
- B. Uncap the Panther Fusion SLT and retain the cap.
- C. Prior to testing on the Panther Fusion system, carefully transfer the determined volume of each individual specimen from the specimen collection container to the Panther Fusion Specimen Lysis Tube.
- D. Ensure homogenous mixing of each prepared sample pool.

**Note:** Retain the individual specimens for additional testing, if required.

**Option 2:****Specimen Preparation Instructions for Samples Pooled Prior to Transferring to a Panther Fusion Specimen Lysis Tube (Panther Fusion SLT)**

Perform the following procedure when pooling specimens collected in VTM/UTM, saline, or Liquid Amies by pooling the samples prior to transferring into a Panther Fusion Specimen Lysis Tube (Panther Fusion SLT).

- A. Obtain a generic empty tube.
- B. Determine the appropriate volume required from each individual specimen based on the pool size being implemented. The required specimen to STM ratio in the assay test sample must be maintained for sample pooling. The minimum combined volume of individual specimens pooled prior to transferring to an SLT is 500 µL. The same volume of each specimen included in the pool needs to be used.

**Note:** it is recommended to prepare > 500 µL of the specimen pool to account for the potential volume loss associated during transfer to the Panther Fusion SLT.

- C. Carefully transfer the determined volume of each individual specimen from the specimen collection container to the generic empty tube.
- D. Uncap the Panther Fusion Specimen Lysis Tube and retain the cap.

- E. Prior to testing on the Panther Fusion system, carefully transfer 500 µL of the combined specimen mixture from the generic tube to the Panther Fusion Specimen Lysis Tube.
- F. Ensure homogenous mixing of each prepared sample pool.

**Note: Retain the individual specimens for additional testing, if required.**

### For Specimens Collected in Aptima Multitest Transport Tubes

Customers may choose from one of the following two options to perform specimen processing for pooled samples using Specimen Lysis Tubes with the Panther Fusion SARS-CoV-2 assay.

#### Option 1:

#### Specimen Preparation Instructions for Samples Pooled Directly into a Panther Fusion Specimen Lysis Tube

Perform the following procedure when pooling specimens collected in Aptima Multitest Transport Tubes by transferring individual specimens directly into a Panther Fusion Specimen Lysis Tube.

- A. Determine the appropriate volume required from each individual specimen based on the pool size being implemented. The required specimen to STM ratio in the assay test sample must be maintained for sample pooling. For example, if a pool size of 5 specimens is being utilized 100 µL of each individual specimen (500 µL total) is required.
- B. Uncap the Panther Fusion Specimen Lysis Tube and retain the cap
- C. Prior to testing on the Panther Fusion system, carefully transfer the determined volume of each individual specimen from the Aptima Multitest Transport Tubes to the Panther Fusion Specimen Lysis Tube.
- D. Ensure homogenous mixing of each prepared sample pool and apply the penetrable cap.

**Note: Retain the individual specimens for additional testing, if required.**

#### Option 2:

#### Specimen Preparation Instructions for Samples Pooled Prior to Transferring to a Specimen Lysis Tube

Perform the following procedure when pooling specimens collected in Aptima Multitest Transport Tubes by pooling the samples prior to transferring into a Specimen Lysis Tube.

- A. Obtain a generic empty tube.
- B. Determine the appropriate volume required from each individual specimen based on the pool size being implemented. The required specimen to STM ratio in the assay test sample must be maintained for sample pooling. The minimum combined volume of individual specimens pooled prior to transferring to an SLT is 500 µL. The same volume of each specimen included in the pool needs to be used.

**Note: it is recommended to prepare > 500 µL of the specimen pool to account for the potential volume loss associated during transfer to the SLT.**

- C. Carefully transfer the determined volume of each individual specimen from the specimen collection container to the generic empty tube.

- D. Uncap the Specimen Lysis Tube and retain the cap.
- E. Prior to testing on the Panther Fusion system, carefully transfer 500 µL of the combined specimen mixture from the generic tube to the Specimen Lysis Tube.
- F. Ensure homogenous mixing of each prepared sample pool.

**Note: Retain the individual specimens for additional testing, if required.**

### Specimen Transport

Maintain specimen storage conditions as described in the *Specimen Collection and Storage* section on page 8.

**Note: Specimens must be shipped in accordance with applicable national, international, and regional transportation regulations.**

## Panther Fusion System

The Panther Fusion System is an integrated nucleic acid testing system that fully automates all steps necessary to perform various Panther Fusion assays from sample processing through amplification, detection, and data reduction.

### Reagents and Materials Provided for the Panther Fusion SARS-CoV-2 Assay

#### Assay Packaging

Components <sup>1</sup>	Part No.	Storage
<b>Panther Fusion Open Access RNA/DNA Enzyme Cartridges 96 Tests</b> Panther Fusion Open Access RNA/DNA cartridge, 12 tests, 8 per box	PRD-04303	2°C to 8°C
<b>Panther Fusion Internal Control-S 960 Tests</b> Panther Fusion Internal Control-S tube, 4 per box	PRD-04332	2°C to 8°C
<b>Panther Fusion SARS-CoV-2 Assay Controls</b> Panther Fusion SARS-CoV-2 Positive Control tube, 5 per box Panther Fusion Negative Control tube, 5 per box	PRD-06404	2°C to 8°C
<b>Panther Fusion Extraction Reagent-S 960 Tests</b> Panther Fusion Capture Reagent-S bottle, 240 tests, 4 per box Panther Fusion Enhancer Reagent-S bottle, 240 tests, 4 per box	PRD-04331	15°C to 30°C
<b>Panther Fusion Elution Buffer 2400 Tests</b> Panther Fusion Elution Buffer pack, 1200 tests, 2 per box	PRD-04334	15°C to 30°C
<b>Panther Fusion SARS-CoV-2 Assay PPR Solution</b> Panther Fusion SARS-CoV-2 Assay PPR Solution tube, 40 tests, 4 per bag	PRD-06391	-15°C to -85°C
<b>Panther Fusion Oil 1920 Tests</b> Panther Fusion Oil pack, 960 tests, 2 per box	PRD-04335	15°C to 30°C
<b>Aptima Oil Reagent</b>	PRD-04304	15°C to 30°C

<sup>1</sup> Components can also be ordered in the following bundles:

Panther Fusion Universal Fluids Kit, PRD-04430, contains 1 each Panther Fusion Oil and Panther Fusion Elution buffer.

Panther Fusion Assay Fluids I-S, PRD-04431, contains 2 Panther Fusion Extraction Reagents-S, 2 Panther Fusion Internal Control-S, and 1 Panther Fusion Reconstitution Buffer I.

#### Individually Packaged Items

Items	Part No.
Panther Fusion Specimen Lysis Tubes, 100 per bag	PRD-04339

## Materials Required and Available Separately

*Note: Materials available from Hologic have catalog numbers listed, unless otherwise specified.*

Material	Cat. No.
Panther System	303095
Panther Fusion Module	ASY-09600
Panther Fusion Open Access Pack	PRD-04305
Aptima Assay Fluids Kit (Aptima Wash Solution, Aptima Buffer for Deactivation Fluid, and Aptima Oil Reagent)	303014 (1000 tests)
Multi-tube units (MTUs)	104772-02
Panther Waste Bag Kit	902731
Panther Waste Bin Cover	504405
Or Panther System Run Kit for Real Time Assays contains MTUs, waste bags, waste bin covers, and assay fluids	PRD-03455 (5000 tests)
Or Panther System Run Kit (when running TMA assays in parallel with real time-TMA assays) contains MTUs, waste bags, waste bin covers, auto detect*, and assay fluids	303096 (5000 tests)
Aptima Multitest Swab Specimen Collection Kit	PRD-03546
Panther Fusion Tube Trays, 1008 tests, 18 trays per box	PRD-04000
Liquid Handling (LiHa) Disposable Tips, 1000 µL	10612513 (Tecan)
Aptima penetrable caps (optional)	105668
Replacement non-penetrable caps (optional)	103036A
Replacement extraction reagent bottle caps	CL0040
P1000 pipettor and tips with hydrophobic plugs	-
Bleach, 5% to 7% (0.7 M to 1.0 M) sodium hypochlorite solution <b>Note:</b> Mix one part bleach with one part deionized water to make diluted working bleach solution 2.5% to 3.5% (0.35 M to 0.5 M) sodium hypochlorite solution.	-
Disposable powderless gloves	-

\*Needed only for Panther Aptima TMA assays.

## Panther Fusion System Test Procedure

**Note:** Refer to the Panther/Panther Fusion System Operator's Manual for additional procedural information.

### A. Work Area Preparation

1. Wipe down work surfaces with 2.5% to 3.5% (0.35 M to 0.5 M) sodium hypochlorite solution. Allow the sodium hypochlorite solution to contact surfaces for at least 1 minute and follow with a deionized (DI) water rinse. Do not allow the sodium hypochlorite solution to dry. Cover the bench surface with clean, plastic-backed absorbent laboratory bench covers.
2. Clean a separate work surface where samples will be prepared using the procedure described in step A.1.

### B. Reagent Preparation

1. Remove the bottles of IC-S, FCR-S and FER-S from storage.
2. Open the bottles of IC-S, FCR-S and FER-S, and discard the caps. Open the TCR door on the upper bay of the Panther Fusion system.
3. Place the IC-S, FCR-S and FER-S bottles in the appropriate positions on the TCR carousel.
4. Close the TCR door.

**Note:** The Panther Fusion system adds the IC-S to the FCR-S. After the IC-S is added to the FCR-S, it is referred to as wFCR-S (working FCR-S). If the FCR-S and FER-S are removed from the system, use new caps and immediately store according to the proper storage conditions.

### C. PPR Solution Preparation

1. Thaw the Panther Fusion SARS-CoV-2 assay PPR Solution to room temperature, protect from light.
2. Mix the solution by vortexing and perform a quick centrifugation to allow contents to settle to the bottom of the tube.
3. Uncap the tube and add 400 µL Aptima Oil Reagent on top of the Panther Fusion SARS-CoV-2 PPR Solution.
4. Recap the tube and perform a quick centrifugation to allow contents to settle to the bottom of the tube and the oil to create an environmental barrier at the top of the tube.
- 5. Uncap PPR tube.**
6. Load 1-4 Panther Fusion SARS-CoV-2 assay PPR Solution tubes with the oil overlay into each Open Access Pack.

**Note:** Do not mix or cool the Panther Fusion SARS-CoV-2 PPR Solution once the oil overlay has been added.

### D. PPR Loading onto Panther Fusion

1. Open the Fusion Universal Fluids Drawer from the Load Universal Fluids option on the Tasks screen or the icon on the bottom of the screen.
2. Place the Open Access Pack with loaded PPR tubes into any open Reconstitution Buffer position.
3. Select "Loaded" for the position(s) in the pack with loaded PPR tubes.

4. Select “set” to select the LDT-SARS-CoV-2 assay from the menu.
5. Confirm that 40 tests have been assigned to the LDT-SARS-CoV-2 tube.
6. Repeat for each PPR tube loaded in the Open Access Pack.
7. Repeat for each additional Open Access Pack containing Panther Fusion SARS-CoV-2 assay PPR Solution tubes until the desired number of tests are loaded.
8. After all tubes are assigned, click Save to complete PPR loading.
9. Gently close the Fusion Universal Fluids Drawer.

#### E. Specimen Handling

**Note:** Prepare specimens per the Specimen Processing instructions in the Specimen Collection and Storage section before loading specimens onto the Panther Fusion system.

1. Inspect sample tubes before loading into the rack. If a sample tube contains bubbles or has a lower volume than is typically observed, gently tap the bottom of the tube to bring contents to the bottom.

**Note:** To avoid a processing error, ensure adequate specimen volume is added to the Panther Fusion Specimen Lysis Tube. When 500  $\mu$ L of collected specimen is added to the Panther Fusion Specimen Lysis Tube, there is sufficient volume to perform 3 nucleic acid extractions.

#### F. System Preparation

For instructions on setting up the Panther Fusion system including loading samples, reagents, assay cartridges and universal fluids, refer to the *Panther/Panther Fusion System Operator's Manual*.

#### G. Load Panther Fusion SARS-CoV-2 Controls onto the Panther Fusion

1. Load the Sample Rack with the Panther Fusion SARS-CoV-2 Negative Control and the Panther Fusion SARS-CoV-2 Positive Control.
2. From the Sample Rack Bay screen, select the rack containing the controls and then Rack Details from the bottom of the screen.
3. Select the tube position in which the Panther Fusion SARS-CoV-2 Negative Control is loaded. The Sample Details screen opens.
4. Select Assign Open Access Control from the bottom of the screen.
5. Select the LDT-SARS-CoV-2 assay under the Assays column and the Negative Control under Control Types.
6. Select Assign.
7. Select the tube position in which the Panther Fusion SARS-CoV-2 Positive Control is loaded. The Sample Details screen opens.
8. Select Assign Open Access Control from the bottom of the screen.
9. Select the LDT-SARS-CoV-2 assay under the Assays column and the SARS-CoV-2 Positive Control under Control Types.
10. Select Assign.



**Procedural Notes**

## A. Controls

1. The Panther Fusion SARS-CoV-2 Positive Control and Panther Fusion SARS-CoV-2 Negative Control tubes can be loaded in any rack position, in any Sample Bay lane on the Panther Fusion system.
2. Once the control tubes are pipetted and are processed for the Panther Fusion SARS-CoV-2 assay, they are active for up to 30 days (control frequency configured by an administrator) unless control results are invalid or a new assay cartridge lot is loaded.
3. Each control tube can be tested once.
4. Patient specimen pipetting begins when one of the following two conditions is met:
  - a. Valid results for the controls are registered on the system.
  - b. A pair of controls is currently in process on the system.

## Quality Control

A run or specimen result may be invalidated by the Panther Fusion System if problems occur while performing the assay. Specimens with invalid results must be retested.

### Negative and Positive Controls

To generate valid results, a set of assay controls must be tested. One replicate of the negative assay control and positive assay control must be tested each time a new lot of assay cartridges or Panther SARS-CoV-2 assay PPR Solution lot is loaded on the Panther Fusion system or when the current set of valid controls have expired.

The Panther Fusion system is configured to require assay controls run at an administrator-specified interval of up to 30 days. Software on the Panther Fusion system alerts the operator when assay controls are required and does not start new tests until the assay controls are loaded and have started processing.

During processing, criteria for acceptance of the assay controls are automatically verified by the Panther Fusion system. To generate valid results, the assay controls must pass a series of validity checks performed by the Panther Fusion system.

If the assay controls pass all validity checks, they are considered valid for the administrator-specified time interval. When the time interval has passed, the assay controls are expired by the Panther Fusion system which requires a new set of assay controls be tested prior to starting any new samples.

If any one of the assay controls fails the validity checks, the Panther Fusion system automatically invalidates the affected samples and requires a new set of assay controls be tested prior to starting any new samples.

### Internal Control

An internal control is added to each sample during the extraction process. During processing, the internal control acceptance criteria are automatically verified by the Panther Fusion system software. Detection of the internal control is not required for samples that are positive for SARS-CoV-2. The internal control must be detected in all samples that are negative for SARS-CoV-2 targets; samples that fail to meet that criteria will be reported as Invalid. Each sample with an Invalid result must be retested.

The Panther Fusion system is designed to accurately verify processes when procedures are performed following the instructions provided in this package insert and the *Panther/Panther Fusion System Operator's Manual*.

## Interpretation of Results

The Panther Fusion system automatically determines the test results for samples and controls. A test result may be negative, positive, or invalid. The Panther Fusion SARS-CoV-2 assay is not a laboratory developed test. The LDT flag associated with reported results does not apply to this test. This assay has been authorized by the FDA under an Emergency Use Authorization.

Table 1 shows the possible results reported in a valid run with result interpretations.

*Table 1: Result Interpretation*

SARS-CoV-2 Result	IC Result	Interpretation
Neg	Valid	SARS-CoV-2 not detected.
POS	Valid	SARS-CoV-2 detected.
Invalid	Invalid	Invalid. There was an error in the generation of the result; retest sample.

Note: POS result will be accompanied by cycle threshold (Ct) values.

Note: Detection of internal control is not required for samples that are positive for SARS-CoV-2.

## Interpretation of Results for Pooled Samples

**Negative**—Negative results from pooled sample testing should not be treated as definitive. If the patient's clinical signs and symptoms are inconsistent with a negative result and if results are necessary for patient management, then the patient should be considered for individual testing. The utilization of sample pooling should be indicated for any specimens with reported negative results.

**Positive**—Specimens with a positive sample pool result must be tested individually prior to reporting a result. Specimens with low viral loads may not be detected in sample pools due to the decreased sensitivity of pooled testing.

**Invalid**—Specimens with an invalid pool result must be tested individually prior to reporting a result. However, in instances of an invalid run, repeat testing of pooled specimens may be appropriate depending on laboratory workflow and required result reporting time.

## Limitations

- A. Use of this assay is limited to personnel who are trained in the procedure. Failure to follow these instructions may result in erroneous results.
- B. Reliable results are dependent on adequate specimen collection, transport, storage, and processing.
- C. Avoid contamination by adhering to good laboratory practices and to the procedures specified in this package insert.
- D. Negative results do not preclude SARS-CoV-2 infections and should not be used as the sole basis for treatment or other management decisions.
- E. A positive result indicates the detection of nucleic acid from the relevant virus. Nucleic acid may persist even after the virus is no longer viable.
- F. Nasal and mid-turbinate nasal swab specimens self-collected under the supervision of or collected by a health care provider and nasopharyngeal wash/aspirate or nasal aspirates are additional acceptable upper respiratory specimens that can be tested with the Panther Fusion SARS CoV- 2 assay; however, performance with these specimen types have not been determined.
- G. Nasopharyngeal wash/aspirate, nasal aspirates, and bronchoalveolar lavage (BAL) specimen types should not be pooled.
- H. Sample pooling has only been validated using nasopharyngeal swab specimens.
- I. Samples should only be pooled when testing demand exceeds laboratory capacity and/or when testing reagents are in short supply.
- J. Use of the Panther Fusion SARS-CoV-2 assay in a general, asymptomatic screening population is intended to be used as part of an infection control plan, that may include additional preventative measures, such as a predefined serial testing plan or directed testing of high-risk individuals. Negative results should be considered presumptive and do not preclude current or future infection obtained through community transmission or other exposures. Negative results must be considered in the context of an individual's recent exposures, history, and presence of clinical signs and symptoms consistent with COVID-19.
- K. Asymptomatic individuals infected with COVID-19 may not shed enough virus to reach the limit of detection of the test, giving a false negative result.
- L. In the absence of symptoms, it is difficult to determine if asymptomatic individuals have been tested too late or too early. Therefore, negative results in asymptomatic individuals may include individuals who were tested too early and may become positive later, individuals who were tested too late and may have serological evidence of infection, or individuals who were never infected.
- M. The performance of this test was established based on the evaluation of a limited number of clinical specimens. Clinical performance has not been established with all circulating variants but is anticipated to be reflective of the prevalent variants in circulation at the time and location of the clinical evaluation. Performance at the time of testing may vary depending on the variants circulating, including newly emerging strains of SARS-CoV-2 and their prevalence, which change over time.

## Conditions of Authorization for Labs

The Panther Fusion SARS-CoV-2 assay Letter of Authorization, along with the authorized Fact Sheet for Healthcare Providers, the authorized Fact Sheet for Patients, and authorized labeling are available on the FDA website: <https://www.fda.gov/medical-devices/coronavirus-disease-2019-covid-19-emergency-use-authorizations-medical-devices/in-vitro-diagnostics-euas>.

However, to assist clinical laboratories using the Panther Fusion SARS-CoV-2 assay, the relevant Conditions of Authorization are listed below.

- A. Authorized laboratories<sup>a</sup> using the Panther Fusion SARS-CoV-2 assay must include with result reports of the Panther Fusion SARS-CoV-2 assay, all authorized Fact Sheets. Under exigent circumstances, other appropriate methods for disseminating these Fact Sheets may be used, which may include mass media.
- B. Authorized laboratories using specimen pooling strategies when testing patient specimens with the authorized test must include with test result reports for specific patients whose specimen(s) were the subject of pooling, a notice that pooling was used during testing and that “Patient specimens with low viral loads may not be detected in sample pools due to the decreased sensitivity of pooled testing.”
- C. Authorized laboratories using the Panther Fusion SARS-CoV-2 assay must use the Panther Fusion SARS-CoV-2 assay as outlined in the authorized labeling. Deviations from the authorized procedures, including the authorized instruments, authorized extraction methods, authorized clinical specimen types, authorized control materials, authorized other ancillary reagents and authorized materials required to perform the Panther Fusion SARS-CoV-2 assay are not permitted.
- D. Authorized laboratories implementing pooling strategies for testing patient specimens must use the “Specimen Pooling Implementation and Monitoring Guidelines” provided in the authorized tests’ Instructions for Use/Package Insert to evaluate the appropriateness of continuing to use such strategies based on the recommendations in the protocol.
- E. Authorized laboratories that receive the Panther Fusion SARS-CoV-2 assay must notify the relevant public health authorities of their intent to run the test prior to initiating testing.
- F. Authorized laboratories using the Panther Fusion SARS-CoV-2 assay must have a process in place for reporting test results to healthcare providers and relevant public health authorities, as appropriate.
- G. Authorized laboratories must collect information on the performance of the test and report to DMD/OHT7-OIR/OPEQ/CDRH (via email: [CDRH-EUA-Reporting@fda.hhs.gov](mailto:CDRH-EUA-Reporting@fda.hhs.gov)) and Hologic (molecularsupport@hologic.com) any suspected occurrence of false positive or false negative results and significant deviations from the established performance characteristics of the test of which they become aware.
- H. All laboratory personnel using the test must be appropriately trained in RT-PCR techniques and use appropriate laboratory and personal protective equipment when handling this kit and use the test in accordance with the authorized labeling.

- I. Hologic, its authorized distributor(s) and authorized laboratories using the Panther Fusion SARS-CoV- 2 assay must ensure that any records associated with this EUA are maintained until otherwise notified by FDA. Such records will be made available to FDA for inspection upon request.
- J. Authorized laboratories must keep records of specimen pooling strategies implemented including type of strategy, date implemented, and quantities tested, and test result data generated as part of the Protocol for Monitoring of Specimen Pooling Strategies. For the first 12 months from the date of their creation, such records will be made available to FDA within 48 business hours for inspection upon request, and will be made available within a reasonable time after 12 months from the date of their creation.

<sup>a</sup> The letter of authorization refers to "Laboratories certified under the Clinical Laboratory Improvement Amendments of 1988 (CLIA), 42 U.S.C. §263a, that meet requirements to perform high complexity tests" as "authorized laboratories."

## Panther Fusion SARS-CoV-2 Assay Performance

### Analytical Sensitivity

The analytical sensitivity (limit of detection or LoD) of the Panther Fusion SARS-CoV-2 assay was determined by testing serial dilutions of pooled negative clinical nasopharyngeal swab specimens spiked with inactivated cultured SARS-CoV-2 virus (USA-WA1/2020; BEI Resources; NR-52281). Ten replicates of each serial dilution were evaluated using two assay reagent lots across two Panther Fusion systems. The LoD was determined to be  $1 \times 10^{-2}$  TCID<sub>50</sub>/mL and verified by testing an additional 20 replicates with one assay reagent lot. The LoD of  $1 \times 10^{-2}$  TCID<sub>50</sub>/mL was also confirmed using saline, Liquid Amies, and specimen transport medium (STM) swab collection media.

A similar analytical sensitivity study was performed using pooled negative clinical bronchoalveolar lavage fluid lower respiratory tract specimens. The LoD was determined and verified to be  $1 \times 10^{-2}$  TCID<sub>50</sub>/mL in the Panther Fusion test sample.

### FDA SARS-CoV-2 Reference Panel Testing

The evaluation of sensitivity and MERS-CoV cross-reactivity was performed using reference material (T1), blinded samples and a standard protocol provided by the FDA. The study included a range finding study and a confirmatory study for LoD. Blinded sample testing was used to establish specificity and to confirm the LoD. The study was performed on the fully automated Panther Fusion system. The results are summarized in Table 2.

Table 2: Summary of LoD Confirmation Results using the FDA SARS-CoV-2 Reference Panel

Reference Materials Provided by FDA	Specimen Type	Product LoD	Cross-Reactivity
SARS-CoV-2	NP Swabs in VTM/UTM	600 NDU/mL	N/A <sub>-</sub>
MERS-CoV		N/A	-ND

NDU/mL = RNA NAAT detectable units/mL.

N/A = Not applicable.

ND = Not detected.

### Inclusivity

The inclusivity of the Panther Fusion SARS-CoV-2 assay was evaluated using *in silico* analysis of the assay primers and probes in relation to 341 SARS-CoV-2 sequences available in the NCBI and GISAID gene databases. Of the 341 sequences, 339 contained information corresponding to both target systems of the assay and 2 contained information corresponding to only one of the two target systems. The *in silico* analysis showed 100% homology to the primers and probes of both target systems for 335 of the evaluated sequences and 100% homology to the primers and probes of at least one target system for the 6 of the evaluated sequences. Five out of the 6 had only one nucleotide mismatch in one oligonucleotide of the second amplification system and were predicted to be reactive.

## Analytical Specificity and Microbial Interference

The analytical specificity of the Panther Fusion SARS-CoV-2 assay was evaluated by testing 26 microorganisms representing common respiratory pathogens or closely related species (Table 3). Bacteria were tested at  $10^6$  CFU/mL and viruses were tested at  $10^5$  TCID<sub>50</sub>/mL, except where noted. Microorganisms were tested with and without the presence of SARS-CoV-2 inactivated virus at 3x LoD. Analytical specificity of the Panther Fusion SARS-CoV-2 assay was 100% with no evidence of microbial interference.

In addition to microorganism testing, *in silico* analysis was performed to assess the specificity of the assay in relation to the microorganisms listed in Table 4. The *in silico* analysis showed no probable cross activity to any of the 183 GenBank sequences evaluated.

Table 3: Panther Fusion SARS-CoV-2 Analytical Specificity and Microbial Interference Microorganisms

Microorganism	Concentration	Microorganism	Concentration
Human coronavirus 229E	1E+5 TCID <sub>50</sub> /mL	Parainfluenza virus 1	8.6E+4 TCID <sub>50</sub> /mL
Human coronavirus OC43	1E+5 TCID <sub>50</sub> /mL	Parainfluenza virus 2	1.5E+4 TCID <sub>50</sub> /mL
Human coronavirus HKU1 <sup>1</sup>	1E+6 copies/mL	Parainfluenza virus 3	1E+5 TCID <sub>50</sub> /mL
Human coronavirus NL63	1E+4 TCID <sub>50</sub> /mL	Parainfluenza virus 4	1E+4 TCID <sub>50</sub> /mL
SARS-coronavirus <sup>1</sup>	1E+6 copies/mL	Influenza A	1E+4 TCID <sub>50</sub> /mL
MERS-coronavirus	2.5E+4 TCID <sub>50</sub> /mL	Influenza B	6E+3 TCID <sub>50</sub> /mL
Adenovirus (e.g. C1 Ad. 71)	1E+5 TCID <sub>50</sub> /mL	Enterovirus (e.g. EV68)	1E+5 TCID <sub>50</sub> /mL
Human Metapneumovirus (hMPV)	1E+6 TCID <sub>50</sub> /mL	Rhinovirus	9.9E+4 TCID <sub>50</sub> /mL
Respiratory syncytial virus	1E+5 TCID <sub>50</sub> /mL	<i>Legionella pneumophila</i>	1E+6 CFU/mL
<i>Chlamydia pneumoniae</i>	5E+6 IFU/mL	<i>Mycobacterium tuberculosis</i>	9.9E+5 TCID <sub>50</sub> /mL
<i>Haemophilus influenzae</i>	1E+6 CFU/mL	<i>Streptococcus pneumoniae</i>	1E+6 CFU/mL
<i>Bordetella pertussis</i>	1E+6 CFU/mL	<i>Streptococcus pyogenes</i>	1E+6 CFU/mL
<i>Pneumocystis jirovecii</i> (PJP)	1E+6 nuc/mL	<i>Mycoplasma pneumoniae</i>	1E+6 CFU/mL
Pooled human nasal wash <sup>2</sup> - to represent diverse microbial flora in human respiratory tract	N/A		

<sup>1</sup> Cultured virus and whole genome purified nucleic acid for Human coronavirus HKU1 and SARS-coronavirus are not readily available. HKU1 and SARS-coronavirus IVTs corresponding to the ORF1ab gene regions targeted by the assay were used to evaluate cross-reactivity and microbial interference.

<sup>2</sup> In place of evaluating pooled human nasal wash, testing of 30 individual negative clinical NP swab specimens was performed to represent diverse microbial flora in the human respiratory tract.



Table 4: *In Silico* Analysis Microorganisms

Microorganism	Number of Strains Evaluated	Microorganism	Number of Strains Evaluated
Human coronavirus 229E	3	<i>Streptococcus pneumoniae</i>	3
Human coronavirus OC43	3	<i>Streptococcus pyogenes</i>	2
Human coronavirus HKU1	3	<i>Bordetella pertussis</i>	3
Human coronavirus NL63	3	<i>Mycoplasma pneumoniae</i>	2
SARS-coronavirus	2	<i>Pneumocystis jirovecii</i> (PJP)	2
MERS-coronavirus	3	Influenza C	1
Adenovirus (e.g. C1 Ad. 71)	17	Parechovirus	24
Human Metapneumovirus (hMPV)	3	<i>Candida albicans</i>	1
Parainfluenza virus 1-4	15	<i>Corynebacterium diphtheriae</i>	7
Influenza A	2	<i>Bacillus anthracis</i> (Anthrax)	2
Influenza B	1	<i>Moraxella catarrhalis</i>	1
Enterovirus (e.g. EV68)	8	<i>Neisseria elongata and meningitidis</i>	4
Respiratory syncytial virus	3	<i>Pseudomonas aeruginosa</i>	2
Rhinovirus	3	<i>Staphylococcus epidermis</i>	2
<i>Chlamydia pneumoniae</i>	3	<i>Streptococcus salivarius</i>	4
<i>Haemophilus influenzae</i>	3	<i>Leptospirosis</i>	10
<i>Legionella pneumophila</i>	4	<i>Chlamydia psittaci</i>	1
<i>Legionella non-pneumophila</i>	24	<i>Coxiella burneti</i> (Q-Fever)	3
<i>Mycobacterium tuberculosis</i>	3	<i>Staphylococcus aureus</i>	3

## Clinical Performance

The clinical performance of the Panther Fusion SARS-CoV-2 assay was evaluated in comparison to a panel of contrived specimens. For the study, a panel of 178 remnant clinical nasopharyngeal specimens was tested using two Panther Fusion SARS-CoV-2 assay reagent lots. All specimens were collected from US patients with signs and symptoms of respiratory infection. The panel consisted of 69 SARS-CoV-2 positive and 109 SARS-CoV-2 negative specimens. Of the 69 positive specimens, 45 were at concentrations 1-2x LoD and 24 were at concentrations 3-5x LoD using inactivated cultured SARS-CoV-2 virus (USA-WA1/2020; BEI Resources; NR-52281) as the target.

The Positive Percent Agreement (PPA) and Negative Percent Agreement (NPA) was calculated in relation to the expected result of the contrived specimen panel, as shown in Table 5. Detection characteristics for positive contrived specimens were calculated by target concentration, as shown in Table 6.

A similar study was performed using a contrived panel of 178 remnant clinical bronchoalveolar lavage fluid lower respiratory tract specimens. Testing was performed using one assay reagent lot and two Panther Fusion systems. The PPA and NPA was calculated in relation to the expected result of the contrived specimen panel, as shown in Table 7. Detection characteristics for positive contrived specimens were calculated by target concentrations, as shown in Table 8.

Table 5: Panther Fusion SARS-CoV-2 Performance Relative to Expected Results for Swab Specimens

		Contrived Specimen Expected Result	
		Positive	Negative
Panther Fusion SARS-CoV-2 Assay	Positive	69	0
	Negative	0	109

Positive Percent Agreement: 100% (94.7% – 100%)

Negative Percent Agreement: 100% (96.6% – 100%)

Overall Agreement: 100% (96.6% – 100%)

Table 6: Panther Fusion SARS-CoV-2 Detection Characteristics for Positive Contrived Swab Specimens

Target Concentration	% Detected	Average SARS-CoV-2 Ct	SARS-CoV-2 Ct % CV
1xLoD	100% (10/10)	35.6	1.9%
1.5xLoD	100% (10/10)	35.0	1.7%
2xLoD	100% (25/25)	34.4	1.3%
3xLoD	100% (9/9)	33.7	0.7%
4xLoD	100% (5/5)	33.4	1.6%
5xLoD	100% (10/10)	33.0	0.6%

Table 7: Panther Fusion SARS-CoV-2 Performance Relative to Expected Results for LRT Specimens

		Contrived Specimen Expected Result	
		Positive	Negative
Panther Fusion SARS-CoV-2 Assay	Positive	70	0
	Negative	0	108

Positive Percent Agreement: 100% (94.8% – 100%)

Negative Percent Agreement: 100% (96.6% – 100%)

Overall Agreement: 100% (97.9% – 100%)

Table 8: Panther Fusion SARS-CoV-2 Detection Characteristics for Positive Contrived LRT Specimens

Target Concentration	% Detected	Average SARS-CoV-2 Ct	SARS-CoV-2 Ct % CV
1xLoD	100% (10/10)	35.6	2.4%
1.5xLoD	100% (10/10)	35.0	1.6%
2xLoD	100% (25/25)	34.5	2.4%
3xLoD	100% (10/10)	33.9	1.5%
4xLoD	100% (5/5)	33.5	1.9%
5xLoD	100% (10/10)	33.1	0.9%

## Clinical Performance in Asymptomatic Individuals

The clinical performance of the Panther Fusion SARS-CoV-2 assay in individuals without signs and symptoms of respiratory infection (asymptomatic individuals) was evaluated in comparison to a high-sensitivity EUA RT-PCR assay. Prospectively collected nasopharyngeal swab specimens collected in viral transport media from US patients were assessed, including 22 specimens positive for SARS-CoV-2 and 180 specimens negative for SARS-CoV-2 using the EUA comparator assay. The PPA and NPA were calculated in relation to the EUA comparator assay results. The PPA and NPA were 95.5% and 98.9%, respectively, for the Panther Fusion SARS-CoV-2 assay in asymptomatic individuals, as shown in Table 9. Ct values for the NP swab samples with positive Panther Fusion SARS-CoV-2 assay results ranged between 16.1 and 38.1 (mean 27.01).

Table 9: Clinical Agreement in NP Swab Specimens from Asymptomatic Individuals

		EUA RT-PCR Assay	
		Positive	Negative
Panther Fusion SARS-CoV-2 Assay	Positive	21	2
	Negative	1	178

Positive Percent Agreement (PPA): 95.5% (78.2% - 99.2%)

Negative Percent Agreement (NPA): 98.9% (96.0% - 99.7%)

Two (2) NP swab samples with false positive results (Ct values 38 and 38.1, respectively) and 1 sample with a false negative result were confirmed negative following retesting with a different high-sensitivity EUA molecular assay. The negative retest results suggest that the 3 discordant NP swab samples had low viral loads.

## Clinical Performance of Pooling up to 5 Specimens

The clinical performance of the Panther Fusion SARS-CoV-2 assay was evaluated in pools consisting of up to 5 specimens. For the study, a pool size of 3 specimens and a pool size of 5 specimens was evaluated. Testing for both pool sizes included positive and negative specimen pools. Each positive specimen pool consisted of one positive specimen with the remaining specimens being negative, whereas the negative specimen pools consisted only of negative specimens. For the pool size of 3 study, 32 positive and 20 negative specimen pools were evaluated. For the pool size of 5 study, 50 positive and 20 negative specimen pools were evaluated. The positive specimens used in the study covered the detectable range of the assay and included low positive specimens (defined as within 1-2 Ct of the assay LoD). Both the pooled and individual specimens were evaluated with the Panther Fusion SARS-CoV-2 assay.

The Positive Percent Agreement (PPA) and Negative Percent Agreement (NPA) were calculated in relation to the expected (individual) result for each evaluated pool size, as shown in Table 10 and Table 11. With a pool size of 5, two of the ten specimens evaluated with target concentrations at or near the LoD of the assay yielded an individual positive result but were not detected as part of a specimen pool.

Scatter plots for the observed individual specimen and pooled specimen Ct values for a pool size of 3 and pool size of 5 are shown in Figure 1 and Figure 2, respectively. With a pool size of 3, a linear relationship was observed between most individual and pooled specimen Ct values, and the observed average shift in Ct of 1.5 between the individual specimens and pooled

specimens aligns to the expected shift. With a pool size of 5, a linear relationship was observed between most individual and pooled specimen Ct values for specimens with an individual result, and the observed average shift in Ct of 2.3 between the individual specimens and pooled specimens aligns to the expected shift. With a pool size of 5, individual specimens at or near the LoD of the assay with a Ct value  $\geq 34.1$  did not show consistent linearity between the individual and pooled specimen Ct values.

An *in silico* analysis of historical data for individual specimens from four geographically distinct customer sites was performed to estimate the expected PPA for a pool size of 3 or a pool size of 5. The *in silico* analysis was performed using the pooling interpretative criteria determined in the pooling clinical study. These criteria are illustrated as line graphs in Figure 3 and Figure 4 respectively. The applied pooling interpretative criteria are as follows: for a pool size of 3, specimens with an individual test Ct value  $< 40.5$  are not expected to be missed, and 100% of specimens with an individual test Ct  $\geq 40.5$  are expected to be missed. For a pool size of 5, specimens with an individual test Ct value  $< 34.1$  are not expected to be missed, 20% of specimens with an individual test Ct value  $\geq 34.1$  and  $< 39.7$  are expected to be missed, and 100% of specimens with an individual test Ct  $\geq 39.7$  are expected to be missed. The results of this analysis are shown in Table 12. Overall,  $\geq 99.7\%$  and  $\geq 94.5\%$  PPA was observed across all sites for a pool size of 3 and pool size of 5, respectively. The results of the *in silico* analysis support 3- and 5-specimen pooling on the Panther Fusion SARS-CoV-2 analysis.

Table 10: Individual and Pooled Specimen Agreement with a Pool Size of 3

		Individual Specimen Result		
		Positive	Negative	Total
Pool of 3 Result	Positive	32	0	32
	Negative	0	20	20
	Total	32	20	52

Positive Percent Agreement: 100.0% (89.3% - 100.0%)

Negative Percent Agreement: 100.0% (83.9% - 100.0%)

Overall Agreement: 100.0% (93.1% - 100.0%)

Table 11: Individual and Pooled Specimen Agreement with a Pool Size of 5

		Individual Specimen Result		
		Positive	Negative	Total
Pool of 5 Result	Positive	47	0	47
	Negative	2	20	22
	Total	49*	20	69

\*One specimen with an invalid individual result was removed from analysis.

Positive Percent Agreement: 95.9% (86.3% - 98.9%)

Negative Percent Agreement: 100.0% (83.9% - 100.0%)

Overall Agreement: 97.1% (90.0% - 99.2%)

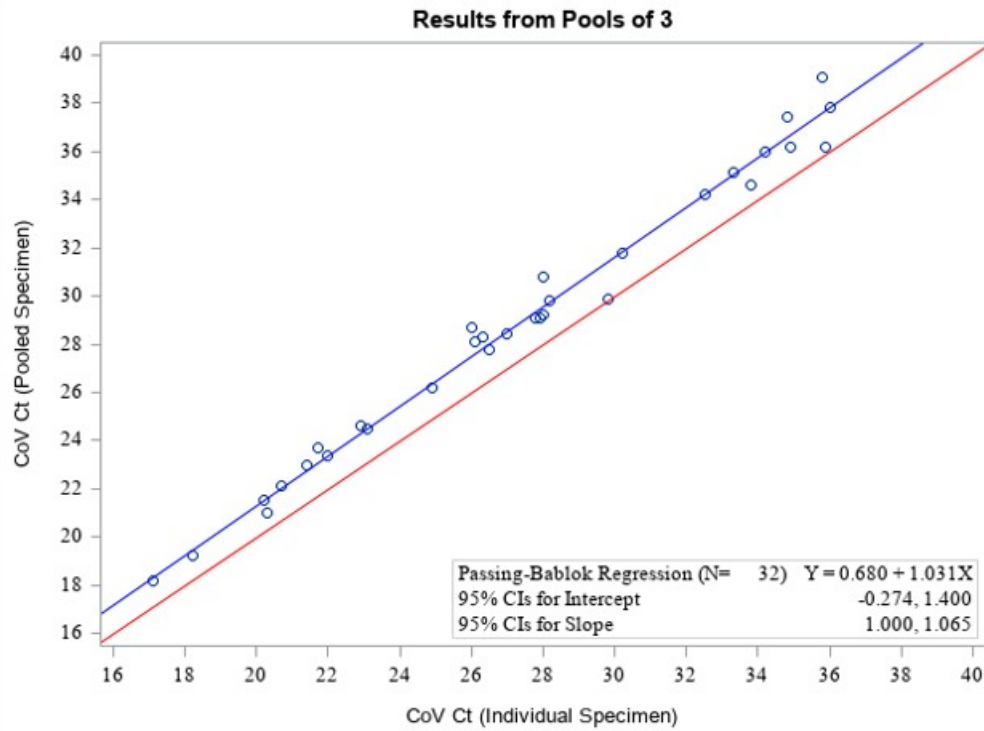


Figure 1. Individual Specimen and Pooled Specimen Ct Scatter Plot for Pool Size of 3

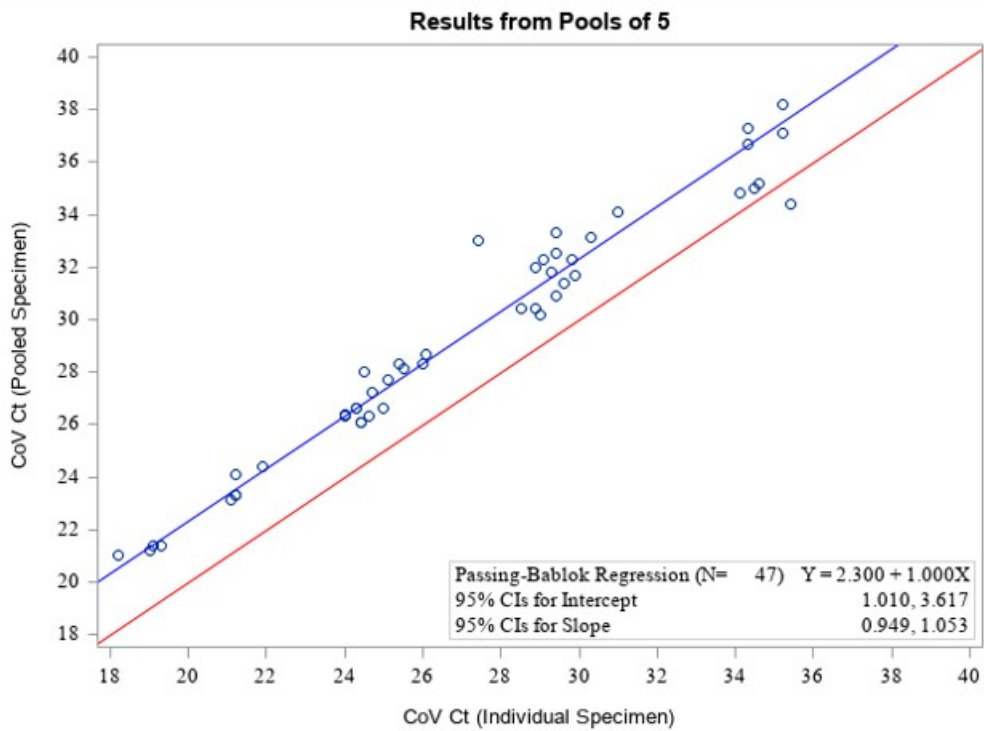


Figure 2. Individual Specimen and Pooled Specimen Ct Scatter Plot for Pooled Size of 5

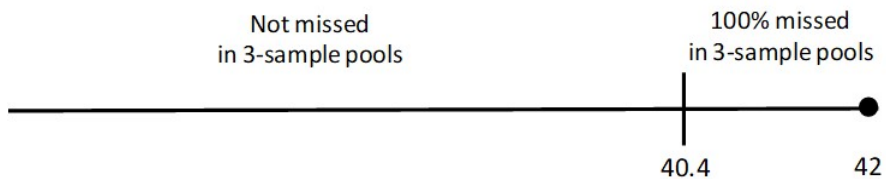


Figure 3. Performance Line Graph for Pool Size of 3

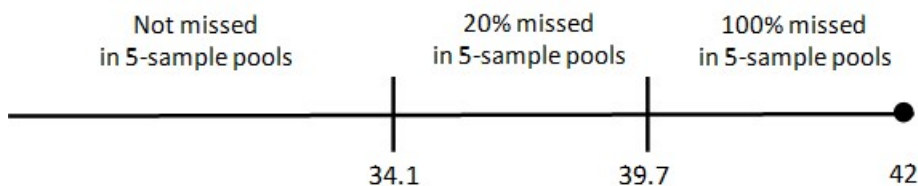


Figure 4. Performance Line Graph for Pool Size of 5

Table 12: In-silico Sensitivity Analysis of Customer Data Set

Site Location	Pool Size of 3			Pool Size of 5		
	N Total	N Positive	PPA (95% C.I.)	N Total	N Positive	PPA (95% C.I.)
New York	28,801	28,780	99.9% (99.9% - 100%)	28,801	27,349.2	95.0% (94.7% - 95.2%)
Utah	1,906	1,900	99.7% (99.3% - 99.9%)	1,906	1811.0	95.0% (93.9% - 95.9%)
California	288	288	100% (98.7% - 100%)	288	272.2	94.5% (91.3% - 96.6%)
Wisconsin	60	60	100% (94.0% - 100%)	60	58.2	97.0% (89.1% - 99.2%)
All Sites	31,055	31,028	99.9% (99.9% - 99.9%)	31,055	29,490.6	95.0% (94.7% - 95.2%)

## Bibliography

1. **World Health Organization.** Q&A on coronaviruses (COVID-19). March 9, 2020. World Health Organization Web site <https://www.who.int/news-room/q-a-detail/q-a-coronaviruses>. Accessed March 10, 2020.
2. **Centers for Disease Control and Prevention.** <https://www.cdc.gov/coronavirus/2019-ncov/prevent-getting-sick/how-covid-spreads.html>. Accessed June 17, 2020.
3. **Centers for Disease Control and Prevention.** Coronavirus Disease 2019-(COVID-19) in the U.S. Updated March 10, 2020. Centers for Disease Control and Prevention Web site <https://www.cdc.gov/coronavirus/2019-ncov/cases-in-us.html>. Accessed March 10, 2020.
4. **Centers for Disease Control and Prevention.** Coronavirus Disease 2019 Information for Travel. Page last reviewed March 8, 2020. Centers for Disease Control and Prevention Web site <https://www.cdc.gov/coronavirus/2019-ncov/travelers/index.html>. Accessed March 10, 2020.
5. **Centers for Disease Control and Prevention.** Coronavirus Disease 2019-(COVID-19) Situation Summary. Updated March 9, 2020. Centers for Disease Control and Prevention Web site <https://www.cdc.gov/coronavirus/2019-ncov/summary.html>. Accessed March 10, 2020.
6. **Clinical & Laboratory Standards Institute.** Document M29 Protection of Laboratory Workers from Occupationally Acquired Infections. CLSI Web site <https://clsi.org/standards/products/microbiology/documents/m29/>. Accessed September 2017.



Hologic, Inc.  
10210 Genetic Center Drive  
San Diego, CA 92121 USA

Customer Support: +1 800 442 9892  
customersupport@hologic.com

Technical Support: +1 888 484 4747  
molecularsupport@hologic.com

For more contact information visit [www.hologic.com](http://www.hologic.com).

Hologic, Aptima, Panther, and Panther Fusion are trademarks and/or registered trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries.

All other trademarks that may appear in this package insert are the property of their respective owners.

This product may be covered by one or more U.S. patents identified at [www.hologic.com/patents](http://www.hologic.com/patents).

©2022 Hologic, Inc. All rights reserved.

AW-21159-001 Rev. 006  
2022-03

## Appendix A: Specimen Pooling Implementation and Monitoring Guidelines

### Before Implementation of Pooling: Determine Appropriate Pool Size

Before a pooling strategy is implemented, a laboratory should determine the appropriate pool size based on percent positivity rate and desired testing efficiency. The Panther Fusion SARS-CoV-2 assay has been validated for n-sample pool sizes up to five samples per pool.

#### If historical laboratory data for individual specimens is available:

- If historical data for individual specimens from the previous 7-10\* days is available, estimate the percent positivity rate ( $P_{\text{individual}}$ ) based on individual results.  

$$(P_{\text{individual}}) = (\text{Number of positive specimen over chosen date range} \div \text{Total number of specimen tested over chosen date range}) * 100.$$
- Using the calculated  $P_{\text{individual}}$  and Table 13, identify the appropriate  $n$  number of samples to pool.
  - If  $P_{\text{individual}}$  is less than 5%, the maximum pool size validated, ( $n=5$ ), should be selected to maximize the efficiency of specimen pooling. Pooling with greater than 5 samples has not been validated and should not be performed.
  - If  $P_{\text{individual}}$  is greater than 25%, Dorfman pooling of patient specimens is not efficient and should not be implemented.

#### If historical laboratory data for individual specimens is unavailable:

- If historical data from the previous 7-10\* days is unavailable, 5, 4, or 3-specimen pooling may still implemented as the Panther Fusion SARS-CoV-2 assay has been validated for 5-specimen pooling.
- Note: without calculating  $P_{\text{individual}}$  and the pooling size implemented may not maximize pooling efficiency.

Table 13: Result Interpretation

<b><i>P</i>, percent of positive subjects in the tested population</b>	<b><i>n</i>maxefficiency (n corresponding to the maximal efficiency)</b>	<b>Efficiency of n-sample pooling (a maximum increase in the number of tested patients when Dorfman n-pooling strategy used)</b>
5%-6%	5	2.15-2.35
7%-12%	4	1.54-1.99
13%-25%	3	1.10-1.48

Because a positive pool requires individual retesting of each sample in the pool, the efficiency of any pooling strategy depends on the positivity rate. The efficiency (F) of n-sample pooling for positivity rate (P) can be calculated with the following formula  $F = 1 / (1 + 1/n - (1-P)^n)$ . The efficiency (F) indicates how many more patients can be tested with n-sample pools compared to individual testing. For example, a 5-sample pooling strategy increases the number of tested patients by 2.15 times for positivity rate P of 6% ( $F=2.15$ ). At  $F=2.15$ , 1,000 tests can on average cover testing of 2,150 patients.



## Implementation of Pooling

See above section titled *Specimen Pooling: Preparing Samples for Pooling* and perform pooling procedure as outlined.

## After Implementation of Pooling: Ongoing Monitoring of Pooling Strategy

### If historical laboratory data for individual specimens is available:

- After implementing a pooling strategy, evaluate the performance of pooled testing by comparing the percent positivity rate of pooled testing to that of individual testing.
- Calculate the percent positivity rate among patient specimens during specimen pooling ( $P_{\text{pools}}$ ) on a daily basis using a moving average of the data from the previous 7-10\* days of testing.  
$$(P_{\text{pools}}) = (\text{Number of patient specimens with a positive result as determined by individual specimen reflex testing of positive pools over chosen date range} \div \text{Total number of patient specimens tested in pools over chosen date range}) * 100$$
- Compare  $P_{\text{pools}}$  to  $P_{\text{individual}}$ . If  $P_{\text{pools}}$  is less than 85% of  $P_{\text{individual}}$ . ( $P_{\text{pools}} < 0.85 \times P_{\text{individual}}$ ), it is recommended that the pool size be reassessed and adjusted to maximize pooling efficiency (if necessary), according to the criteria in Table 12.
- To ensure maximum pooling efficiency, it is recommended that  $\eta_{\text{maxefficiency}}$  be reassessed periodically while sample pooling is implemented by the laboratory.

### If historical laboratory data for individual specimens is unavailable:

- After initiating a pooling strategy, evaluate the performance of pooled testing by calculating the initial percent positivity rate for pooled specimens ( $P_{\text{pools-initial}}$ ). ( $P_{\text{pools-initial}}$  is the percent positivity rate for pooled specimens for the first 7-10\* days of pooled testing.
- Calculate the initial percent positivity rate for individual specimens from pool testing ( $P_{\text{pools-initial}}$ ) from the first 7-10\* days of testing.  
$$P_{\text{pools-initial}} = (\text{Number of patient specimens with a positive result as determined by individual specimen reflex testing of positive pools in first 7-10* days} \div \text{Total number of patient specimens tested in pools in the first 7-10* days}) * 100$$
  - If  $P_{\text{pools-initial}}$  is greater than 25%, pooling of patient specimens is not efficient and should be discontinued until the percent positivity rate decreases.
  - If  $P_{\text{pools-initial}}$  is less than or equal to 25%, pooling of patient specimens can be continued.
- Continue to monitor pooling strategy by calculating the percent positivity rate among patient specimens during specimen pooling ( $P_{\text{pools-x}}$ ) for subsequent 7-10\* day periods. ( $P_{\text{pools-x}}$ ) should be updated daily using a moving average.

- Compare  $P_{\text{pools-x}}$  to  $P_{\text{pools-initial}}$ . If  $P_{\text{pools-x}}$  is less than 90% of  $P_{\text{pools-initial}}$  ( $P_{\text{pools-x}} < 0.90 \times P_{\text{pools-initial}}$ ), it is recommended that the pool size be reassessed and potentially adjusted to maximize pooling efficiency.
- To ensure maximum pooling efficiency, it is recommended that  $\eta_{\text{maxefficiency}}$  be reassessed periodically while sample pooling is implemented by the laboratory.

\*7-10 days is recommended for calculating  $P_{\text{individual}}$ ,  $P_{\text{pools}}$ ,  $P_{\text{pools-initial}}$ , and  $P_{\text{pools-x}}$ . Laboratories should determine if 7-10 days is appropriate by taking into consideration laboratory testing volume and percent positivity. If the number of individual or pooled positive results collected during a given time frame is less than 10,  $P_{\text{individual}}$ ,  $P_{\text{pools}}$ ,  $P_{\text{pools-initial}}$ , and  $P_{\text{pools-x}}$  may not be representative of the percent positivity in the testing population. Consider extending the data collection time period to increase the number of positives evaluated.

# Aptima® Multitest Swab Specimen Collection Kit

**US Only: For Emergency Use Authorization (EUA) Only**

**Rx Only**

**IVD**

## Instructions for SARS-CoV-2 Specimen Collection

The Aptima® Multitest Swab Specimen Collection Kit is intended to be used for clinician collection of oropharyngeal and anterior nasal (nasal) swab specimens and patient collection of nasal swab specimens in a health care setting for testing with the Aptima® SARS-CoV-2 assay and Panther Fusion® SARS-CoV-2 assay to detect the presence of RNA for SARS-CoV-2. The kit is also intended to be used for clinician collection of nasal swab specimens and patient collection of nasal swab specimens in a health care setting for testing with the Aptima® SARS-CoV-2/Flu assay to detect the presence of RNA for SARS-CoV-2, influenza A virus (Flu A), and/or influenza B virus (Flu B). The Aptima Multitest Swab Specimen Collection Kit has not been evaluated for home use.

## Warnings and Precautions

- A. Wash hands with soap before opening collection kit.
- B. Use the provided swab only. Failure to use the provided swab may invalidate the test results.
- C. Do not use if the swab is visibly damaged (i.e., if the swab tip or shaft is broken or pouch is damaged or open).
- D. Do not bend or shape the swab before collection. Do not use excessive force, pressure or bending when collecting the specimen as this may result in accidental breakage of the swab.
- E. Do not apply the specimen transport medium directly to skin or mucous membranes or take internally.
- F. Specimens may be infectious. Use Universal Precautions when handling specimens. Only personnel adequately trained in handling infectious materials should be permitted to handle specimens.
- G. This product has not been FDA cleared or approved for use with the Aptima SARS-CoV-2 assay, Aptima SARS-CoV-2/Flu assay, and Panther Fusion SARS-CoV-2 assay, but has been authorized for emergency use by FDA under an EUA for use by authorized laboratories.
- H. When used with the Aptima SARS-CoV-2 assay and/or Panther Fusion SARS-CoV-2 assay the following applies: This product is for use with a test authorized only for the detection of nucleic acid from SARS-CoV-2, not for any other viruses or pathogens.
- I. When used with the Aptima SARS-CoV-2/Flu assay the following applies: This product is for use with a test authorized only for the detection of nucleic acid from SARS-CoV-2, Flu A, and/or Flu B, not for any other viruses or pathogens.
- J. The emergency use of this product is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of *in vitro* diagnostics for detection

and/or diagnosis of COVID-19 under Section 564(b)(1) of the Federal Food, Drug and Cosmetics Act, 21 U.S.C. § 360bbb-3(b)(1), unless the declaration is terminated or authorization is revoked sooner.

- K. Take care to avoid cross-contamination during the specimen handling steps. Specimens can contain extremely high levels of pathogens. Ensure that specimen containers do not contact one another, and discard used materials without passing over the containers. If gloves come in contact with specimen, change gloves to avoid cross-contamination.
- L. If the contents of the transport tube are spilled at any time during the collection procedure, use a new Aptima Multitest Swab Specimen Collection Kit. Failure to use a new kit may invalidate the test results.
- M. Maintain proper storage conditions during specimen shipping to ensure the integrity of the specimen. Specimen stability under shipping conditions other than those recommended has not been evaluated.
- N. Do not use the kit after its expiration date to collect specimens.

## Kit Storage Requirements

Store collection kit at room temperature (15°C to 30°C).

## Multitest Swab Specimen Performance

Assay performance characteristics using the Multitest swab specimens are provided in the Aptima SARS-CoV-2 assay package insert, Aptima SARS-CoV-2/Flu assay package insert, and Panther Fusion SARS-CoV-2 assay package insert. Package inserts for the Aptima SARS-CoV-2 assay, Aptima SARS-CoV-2/Flu assay, and Panther Fusion SARS-CoV-2 assay may be referenced online at [www.hologic.com](http://www.hologic.com).

When collecting multiple specimens from the same patient, the tube label provides a specimen source field for unique identification of each specimen.

## Oropharyngeal Swab Specimens Collection and Handling – Aptima SARS-CoV-2 Assay and Panther Fusion SARS-CoV-2 Assay

Instructions for oropharyngeal swab specimen collection (clinician collection only):

1. Partially peel open the swab package. Remove the swab. Do not touch the soft tip or lay the swab down. If the soft tip is touched, the swab is laid down, or the swab is dropped, use a new Aptima Multitest Swab Specimen Collection Kit.
2. Hold the swab, placing your thumb and forefinger in the middle of the swab shaft covering the score line. Do not hold the swab shaft below the score line.
3. Carefully insert the swab into the throat ensuring contact with bilateral tonsils (if present) and the posterior pharyngeal wall, then withdraw the swab without touching the inside of the cheeks or tongue.
4. While holding the swab in the same hand, unscrew the cap from the tube. Do not spill the contents of the tube. If the contents of the tube are spilled, use a new Aptima Multitest Swab Specimen Collection Kit.
5. Immediately place the swab into the transport tube so that the score line is at the top of the tube.
6. Carefully break the swab shaft at the score line against the side of the tube.
7. Immediately discard the top portion of the swab shaft.
8. Tightly screw the cap onto the tube.

## Nasal Swab Specimens Collection and Handling – Aptima SARS-CoV-2 Assay, Aptima SARS-CoV-2/Flu Assay, and Panther Fusion SARS-CoV-2 Assay

**Note to Patient:** If you have any questions about this procedure, please ask your healthcare provider.

### Instructions for nasal swab specimen collection: clinician collection and patient self-collection

1. Wash hands with soap and water for 30 seconds before starting.
2. Partially peel open the swab package. Remove the swab. Do not touch the soft tip or lay the swab down. If the soft tip is touched, the swab is laid down, or the swab is dropped, use a new Aptima Multitest Swab Specimen Collection Kit.
3. Hold the swab, placing your thumb and forefinger in the middle of the swab shaft covering the score line. Do not hold the swab shaft below the score line.




4. Carefully insert the swab into the first nostril until the swab tip is no longer visible, i.e.  $\frac{1}{2}$  to  $\frac{3}{4}$  of an inch or 1.25 to 2 cm into the nostril. Rotate the swab with moderate pressure against as much of the wall of the nostril as possible in a large circular path inside the nose at least 4 times (approximately 10-15 seconds per nostril) against the nasal wall and remove from nostril.

**Note:** Simply twirling the swab against one part of the inside of the nose or leaving the swab in the nose for 10-15 seconds, is not proper technique and may result in an insufficient sample.

5. Using the same swab, carefully insert the swab into the second nostril until the swab **tip** is no longer visible, i.e.,  $\frac{1}{2}$  to  $\frac{3}{4}$  of an inch or 1.25 to 2 cm into the nostril. Rotate the swab with moderate pressure against as much of the wall of the nostril as possible in a large circular path inside the nose at least 4 times (approximately 10-15 seconds per nostril) and remove from nostril. **Do not force the swab any further up and into nose at any point.**

**Note:** You must collect the sample from both nostrils!

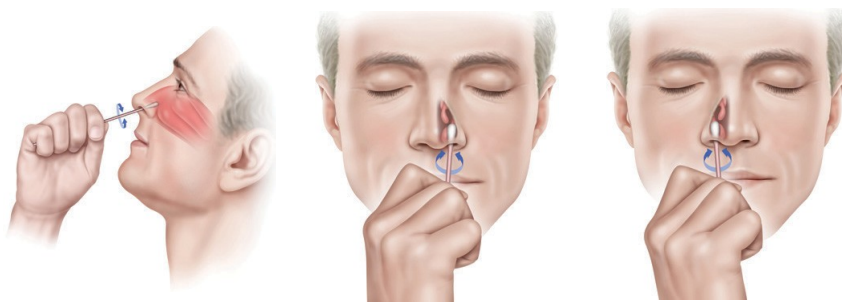

6. While holding the swab in the same hand, unscrew the cap from the tube. Do not spill the contents of the tube. If the contents of the tube are spilled, use a new Aptima Multitest Swab Specimen Collection Kit.

**Note to Patient:** Inform your doctor or healthcare worker if liquid is spilled and a new kit is required.

**Warning: If you come into contact with liquid from the tube, wash your hands with soap and water for 30 seconds.**

7. Immediately place the swab into the transport tube so that the score line is at the top of the tube.
8. Carefully break the swab shaft at the score line against the side of the tube.
9. Immediately discard the top portion of the swab shaft.
10. Tightly screw the cap onto the tube.

**Note:** Simply twirling the swab against one part of the inside of the nose or leaving the swab in the nose for 10-15 seconds, is not proper technique and may result in an insufficient sample.

**Note to Patient:** Return the collection kit to your doctor or healthcare worker.

## Specimen Transport and Storage

Multitest swab specimens are intended to be transported to the laboratory in the provided swab specimen transport medium and tube for use with the Aptima SARS-CoV-2 assay, Aptima SARS-CoV-2/Flu assay, and Panther Fusion SARS-CoV-2 assay. Refer to the Aptima SARS-CoV-2 assay package insert, Aptima SARS-CoV-2/Flu assay package insert, and Panther Fusion SARS-CoV-2 assay package insert for proper specimen storage conditions.

**Note:** Specimens must be shipped in accordance with applicable national and international regulations.

## Limitations

- A. Use this collection kit only with the Aptima SARS-CoV-2 assay, Aptima SARS-CoV-2/Flu assay, Panther Fusion SARS-CoV-2 assay, and other Hologic products. Performance has not been established with other products.
- B. Use appropriate personal protective equipment (PPE) when collecting and handling specimens from individuals suspected of being infected with SARS-CoV-2 as outlined in CDC Interim Laboratory Biosafety Guidelines for Handling and Processing Specimens Associated with 2019 Novel Coronavirus (2019-nCoV).
- C. The patient-collected Aptima Multitest Swab Specimen Collection Kit nasal swab application is limited to health care facilities where support/counseling is available to explain the procedures and precautions.
- D. Oropharyngeal swabs are authorized for use with the Aptima SARS-CoV-2 assay and Panther Fusion SARS-CoV-2 assay only.



Hologic, Inc.  
10210 Genetic Center Drive  
San Diego, CA 92121 USA



**Hologic BV**  
Da Vincilaan 5  
1930 Zaventem  
Belgium

For country-specific Technical Support and Customer Service email address and telephone number, visit [www.hologic.com/support](http://www.hologic.com/support).

Hologic, Aptima, Panther Fusion, and associated logos, are trademarks and/or registered trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries.

All other trademarks that may appear in this document are the property of their respective owners.

This product may be covered by one or more U.S. patents identified at [www.hologic.com/patents](http://www.hologic.com/patents).

©2016-2022 Hologic, Inc. All rights reserved.

2022-01

# Panther Fusion®

REF PRD-06391

SARS-CoV-2  
Primer Probe Reagent Mix



For Use Under an Emergency  
Use Authorization (EUA) Only



(01) 15420045513440

(17) 250715

(10) 123456PV

**LOT** 123456PV



2025-07-15

- Rx Only
- For *in vitro* diagnostic use
- For use under an Emergency Use Authorization (EUA) only
- This product has not been FDA cleared or approved, but been authorized for emergency use by FDA under an EUA for use by authorized laboratories.
- This product has been authorized only for the detection of nucleic acid from SARS-CoV-2, not for any other viruses or pathogens.
- The emergency use of this product is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of *in vitro* diagnostics for detection and/or diagnosis of COVID-19 under Section 564(b)(1) of the Federal Food, Drug, and Cosmetic Act, 21 U.S.C. § 360bbb-3(b)(1), unless the declaration is terminated, or authorization is revoked sooner.
- The current electronic instructions for use are available at <https://www.hologic.com/package-inserts>
- To request a paper copy of the instructions for use free of charge, please contact Hologic Technical Support at [molecularsupport@hologic.com](mailto:molecularsupport@hologic.com)



Hologic, Inc.

10210 Genetic Center Drive  
San Diego, CA 92121 USA

AW-21280 Rev. 002