

STANDARD M nCoV Real-Time Detection kit

For Use Under the Emergency Use Authorization (EUA) Only

Instructions for Use (IFU)



For *in vitro* diagnostic use



For prescription use only



For Use only under Emergency Use Authorization



M-NCOV-01



96 Tests



-25°C ~ -15°C



SD BIOSENSOR, Inc.

C-4th&5th, 16, Deogyong-daero 1556beon-gil, Yeongtong-gu, Suwon-si,
Gyeonggi-do, 16690, REPUBLIC OF KOREA

- Contents -

1. Introduction	3
2. Intended Use.....	3
3. Principle of the Procedure	3
4. Kit Contents	4
5. Storage and Stability Conditions	4
6. Compatible Instruments	4
7. Additionally Required Materials and Equipment	4
8. Description of Symbols	5
9. Warnings and Precautions	5
10. Reagent Handling	9
11. Good Laboratory Practice	9
12. Procedure	9
13. Quality Control	10
14. Limitations of the Kit Protocols	11
15. Conditions of Authorization	12
16. Non-clinical Performance Evaluation.....	13
17. Clinical Performance Evaluation.....	18
18. Troubleshooting	19
19. Reference	19

1. Introduction

Coronavirus is a single-stranded positive-sense RNA virus with an envelope of about 80 to 120 nm in diameter. Its genetic material is the largest of all RNA viruses and is an important pathogen of many domestic animals, pets, and human diseases. It can cause a variety of acute and chronic diseases. Common signs of a person infected with a coronavirus include respiratory symptoms, fever, cough, shortness of breath, and dyspnea. In more severe cases, infection can cause pneumonia, severe acute respiratory syndrome, kidney failure, and even death. The 2019 new coronavirus, or "SARS-CoV-2", was discovered because of Wuhan Viral Pneumonia cases in 2019, and was named by the World Health Organization on January 12, 2020, confirming that it can cause colds and the Middle East Respiratory Syndrome (MERS) and more serious diseases such as acute respiratory syndrome (SARS). This kit is helpful for the auxiliary diagnosis of SARS-CoV-2 infection. The test results are for clinical reference only and cannot be used as a basis for confirming or excluding cases alone.

2. Intended Use

The STANDARD M nCoV Real-Time Detection kit is a real-time reverse transcription-PCR assay for the qualitative detection of SARS-CoV-2 nucleic acids in nasopharyngeal, oropharyngeal, nasal, and mid-turbinate nasal swab, and sputum specimens from individuals who are suspected of COVID-19 by their healthcare provider. Testing is limited to laboratories certified under the Clinical Laboratory Improvement Amendments of 1988 (CLIA), 42 USC §263a, to perform high complexity tests.

Results are for the identification of SARS-CoV-2 RNA. The SARS-CoV-2 RNA is generally detectable in upper respiratory specimens during the acute phase of infection. Positive results are indicative of the presence of SARS-CoV-2 RNA; clinical correlation with patient history and other diagnostic information is necessary to determine patient infection status. Positive results do not rule out bacterial infection or co-infection with other viruses. The agent detected may not be the definite cause of disease. Laboratories within the United States and its territories are required to report all positive results to the appropriate public health authorities.

Negative results do not preclude SARS-CoV-2 infection and should not be used as the sole basis for patient management decisions. Negative results must be combined with clinical observations, patient history, and epidemiological information.

The STANDARD M nCoV Real-Time Detection kit is intended for use by qualified and trained clinical laboratory personnel specifically instructed and trained in the techniques of real-time PCR and *in vitro* diagnostic procedures. The STANDARD M nCoV Real-Time Detection kit is only for use under the Food and Drug Administration's Emergency Use Authorization.

3. Principle of the Procedure

STANDARD M nCoV Real-Time Detection kit is designed according to "WHO interim guidance for laboratory testing for 2019 novel coronavirus (2019-nCoV) in humans". This kit is based on TaqMan probe real-time fluorescent PCR technology. Coronavirus RNA was first transcribed into cDNA by reverse transcriptase, and then cDNA was used as a template for PCR amplification. During the PCR reaction, the 5'→ 3' polymerase activity of Taq DNA polymerase and exo-nuclease were simultaneously used. Dicer activity, which causes the degradation of the TaqMan probe, and the separation of the fluorophore and quencher makes the fluorescence signal detected by the instrument: FAM channel qualitative detection of the new coronavirus (SARS-CoV-2) ORF1ab (RdRp) gene, JOE (VIC or HEX) channel qualitative detection of the coronavirus E gene, and CY5 channel detection internal reference. The kit uses dUTP and UNG enzymes to prevent contamination of amplification products.


STANDARD M nCoV Real-Time Detection kit

Target	Channel
ORF1ab (RdRp) gene	FAM
E gene	JOE (VIC or HEX)
Internal control (IC)	CY5

4. Kit Contents

This kit is used for 96 test / kits. The kit contents are as follows;

	Reagent	Quantity	Volume in each reaction
1	2019-nCoV Reaction Solution	750 μ l/vial x 2	14 μ l
2	RTase Mix	630 μ l/vial x 1	6 μ l
3	2019-nCoV Positive control	600 μ l/vial x 1	-
4	Negative control	600 μ l/vial x 1	-
5	Internal control A	525 μ l/vial x 1	5 μ l (as extraction control) 0.5 μ l (as internal control)
6	ROX	55 μ l/vial x 1	0.5 μ l
7	Instructions for use	1	-

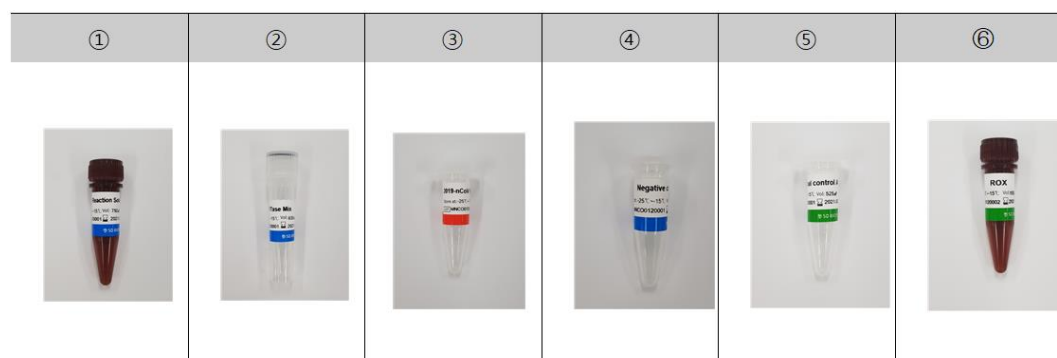

5. Storage and Stability Conditions

1. The kit should be shipped and stored at the temperature of -25°C(-13°F) to -15°C(5°F).
2. The components of 2019-nCoV Reaction Solution and ROX should be stored away from light.
3. Kit materials are stable until the expiration date printed on the outer packaging.
4. Freeze-thawing of kit components more than 5 times may lead to inaccurate results.
5. Dispose of unused reagents and waste in accordance with country, federal, state, and local regulations.

6. Compatible Instruments
















- LightCycler® 480 (S/W version 1.5.1.62, Roche)
- CFX96™ Dx System (S/W version 3.1, Bio-Rad)
- Applied Biosystems 7500 Real-Time PCR Instrument System (S/W version 2.0.6, Thermo Fisher Scientific)

7. Additionally Required Materials and Equipment

- Disposable latex gloves
- Sterilized filtered pipette tips
- Pipettes
- Sterilized (DNase, RNase free) micro centrifuge tube (1.5ml)

- Nucleic acid extraction kit (QIAamp® Viral RNA Mini Kit, Qiagen, Cat.no. 52904)
- Vortex mixer
- Desktop centrifuge
- Clean bench
- RNase neutralizing agent
- Flake or snow type ice
- Thermal cycler
- 0.2ml PCR strips, plate (DNase, RNase free) and cap or sealing film for each Real-time PCR equipment
- PPE (Personal Protective Equipment)
- Biohazard waste container

8. Description of Symbols

Symbol	Description
	<i>In vitro</i> diagnostic medical device
	For prescription use only
	For Use only under Emergency Use Authorization
	Reference number
	Contains sufficient for <n> tests
	Temperature limit
	Manufacturer
	Use-by date
	Batch code
	Date of Manufacture
	Caution
	Instructions for use
	Fulfill the requirements of Directive 98/79/EC on <i>in vitro</i> diagnostic medical devices
	Authorized representative in the European Community
	Fulfill the requirements of KGMP

9. Warnings and Precautions

- Federal Law restricts this device to sale by or on the order of a licensed practitioner.
- This kit is only for *in vitro* diagnostics only.
- Please read the instructions for use carefully before testing.
- All instruments used in the experiment should be sterilized.
- Do not eat, drink, smoke, apply cosmetics or handle contact lenses in areas where reagents and human specimens are handled.
- Handle all specimens as if infectious using safe laboratory procedures. Refer to Interim Laboratory Biosafety Guidelines for Handling and Processing Specimens Associated with 2019-nCoV <https://www.cdc.gov/coronavirus/2019-nCoV/lab-biosafety-guidelines.html>. Dispose of hazardous or biologically contaminated materials according to the practices of your institution.
- Improper specimen collection, transfer, storage, and processing may cause erroneous test results.
- Nucleic acid extraction should be performed as soon as possible after specimen collection to avoid viral nucleic acid degradation; if it cannot be performed as soon as possible, it should be stored in accordance with SPECIMEN COLLECTION AND PREPARATION.
- After the operation of the nucleic acid extraction instrument, the used consumables should be sealed. After the instrument is cleaned, turn on the UV lamp for 30 minutes.
- As this test involves extraction of viral RNA and PCR amplification, care should be taken to avoid contamination of the amplification reaction mixture of the kit. Regular monitoring of laboratory contamination is recommended.
- Clinical laboratories should be equipped with equipment and operators in strict accordance with the "Code of Practice for Clinical Gene Amplification Laboratories".
- When using this kit, it should be operated strictly in accordance with the instructions; the specimen processing and specimen addition steps must be performed in a biological safety cabinet or other basic protective facilities, and follow the technical requirements of the clinical gene amplification laboratory.

10. Reagent Handling

- Handle all reagents, controls, and samples according to good laboratory practice in order to prevent carryover of samples or controls.
- Before use, visually inspect each reagent to ensure that there are no signs of leakage. If there is any evidence of leakage, do not use that material for testing.
- STANDARD M nCoV Real-Time Detection kit Reagent contains guanidine thiocyanate, a potentially hazardous chemical. Avoid contact of reagents with the skin, eyes, or mucous membranes. If contact does occur, immediately wash with generous amounts of water; otherwise, burns can occur.
- Avoid contact of reagents with the skin, eyes, or mucous membranes. If contact does occur, immediately wash with generous amounts of water; otherwise, burns can occur. If these reagents are spilled, dilute with water before wiping dry.
- Dispose of all materials that have come in contact with samples and reagents in accordance with country, state, and local regulations.

11. Good Laboratory Practice

- Do not pipette by mouth.
- Do not eat, drink, or smoke in designated work areas.
- Wear laboratory gloves, laboratory coats, and eye protection when handling samples and reagents. Gloves must be changed between handling samples and STANDARD M nCoV Real-Time Detection kits. Prevent contamination. Avoid contaminating gloves when handling samples and controls.
- Wash hands thoroughly after handling samples and kit reagents, and after removing the gloves.
- Thoroughly clean and disinfect all laboratory work surfaces with a freshly prepared solution of 0.5% sodium hypochlorite in distilled or deionized water (dilute household bleach 1:10). Follow by wiping the surface with 70% ethanol.

12. Procedure

12.1. Specimen collection and preparation

Refer to CDC Interim Guidelines for Collecting, Handling, and Testing Clinical Specimens from Persons Under Investigation (PUIs) for Coronavirus Disease 2019 (COVID-19) (<https://www.cdc.gov/coronavirus/2019-nCoV/lab/guidelines-clinical-specimens.html>)

1) Specimen collection

[Nasopharyngeal swab]

1. Hold the nasopharyngeal swab close to the nasal septum slowly and deeply to the back of the nasopharynx.
2. Rotate it several times to obtain secretions.
3. Quickly dip the swab into the specimen collection tube, and discard the tail.
4. Tighten the tube cap to seal in case of drying.
5. Label the transport tube with sample identification information, including date of collection.

[Oropharyngeal swab]

1. Use moderate swab to wipe the posterior wall of the pharynx and the tonsils on both sides avoiding touching the tongue.
2. Quickly dip the swab into the specimen collection tube, and discard the tail.
3. Tighten the tube cap to seal in case of drying.
4. Label the transport tube with sample identification information, including date of collection.

[Nasal mid-turbinate (NMT) swab, also called Deep Nasal Swab]

1. Use a flocked tapered swab. Tilt patient's head back 70 degrees. While gently rotating the swab, insert swab less than one inch (about 2 cm) into nostril (until resistance is met at turbinates).
2. Rotate the swab several times against nasal wall and repeat in other nostril using the same swab.
3. Quickly dip the swab into the specimen collection tube, and discard the tail.
4. Tighten the tube cap to seal in case of drying.
5. Label the transport tube with sample identification information, including date of collection.

[Anterior nares specimen (NS)]

1. Using a flocked or spun polyester swab, insert the swab at least 1 cm (0.5 inch) inside the nares and firmly sample the nasal membrane by rotating the swab and leaving in place for 10 to 15 seconds. Sample both nares with same swab.
2. Quickly dip the swab into the specimen collection tube, and discard the tail.
3. Tighten the tube cap to seal in case of drying.
4. Label the transport tube with sample identification information, including date of collection.

[Sputum]

1. Collect sputum specimen by inducing a cough into a sterile container.
2. Specimens should be taken carefully to avoid contamination and completely sealed to prevent leakage during transportation (Triple packaging).
3. Label the transport tube with sample identification information, including date of collection.

2) Specimen storage

Specimens can be stored at 2-8°C (35.6-46.4°F) for up to 72 hours after collection. If a delay in testing or shipping is expected, store specimens at -70°C (-94°F) or below.

3) Specimen transport

Specimens must be packaged and transported in accordance with the International Air Transport Association (IATA) Dangerous Goods Regulation. Follow shipping regulations for UN 3373 Biological Substance, Category B when sending potential SARS-CoV-2 specimens

12.1. Assay Protocol

[Nucleic Acid Extraction]

The QIAamp Viral RNA mini kit (QIAGEN, Cat. No. 52904) is used for nucleic acid extraction of specimens and reference materials.

1. The specimen volume required for nucleic acid extraction is 200µℓ.
2. When IC is used for extraction control, add 5µℓ of internal control A to each specimen to be extracted (including positive and negative controls)
3. After the nucleic acid extraction is completed, each eluent should be added to a reaction well immediately.

[Reagent Preparation]

1. LightCycler 480 or CFX96™ Dx System
Prepare the PCR mixture according to the table below for N reactions plus the PC and NC and dispense 20µℓ into each PCR reaction tube.

#	Reagents	Dosage in each reaction
1	2019-nCoV Reaction Solution	N x 14µℓ
2	RTase Mix	N x 6µℓ
3	Internal control A [‡]	N x 0.5µℓ
Total volume/well		20µℓ

[‡] If the IC (Internal Control A) is not used as an extraction control, add 0.5µℓ of IC into PCR master mix per 1 reaction and dispense 20.5µℓ into each well.

NOTE: PCR reaction mixture can be stored below 8°C (46.4°F) for 3 hours.

STANDARD M nCoV Real-Time Detection kit

2. Applied Biosystems 7500 Real-Time PCR Instrument System

Prepare the PCR mixture according to the table below and dispense 20.5µℓ into each PCR reaction tube.

	Reagents	Dosage in each reaction
1	2019-nCoV Reaction Solution	N x 14µℓ
2	RTase Mix	N x 6µℓ
3	ROX	N x 0.5µℓ
4	Internal control A [‡]	N x 0.5µℓ
Total volume/well		20.5µℓ

[‡] If the IC (Internal Control A) is not used as an extraction control, add 0.5µℓ of IC into PCR master mix per 1 reaction and dispense 21µℓ into each well.

NOTE: PCR reaction mixture can be stored below 8°C (46.4°F) for 3 hours.

[RT-PCR Amplification]

1. Add 10µℓ of each of the negative control, positive control, and patient sample nucleic acid extract to the PCR mixture dispensed in each reaction tube.
2. Centrifuge at low speed for a few seconds, and place them on the real-time fluorescence quantitative PCR instrument.
3. Set the cycle conditions below on the PCR instrument.

Reaction	Temp. (°C)	Time	Cycle
Reverse transcription	50°C(122°F)	15 minutes	1
Initial denaturation	95°C(203°F)	3 minutes	1
Pre-amplification	95°C(203°F)	5 seconds	5
	60°C(140°F)	40 seconds	
Amplification	95°C(203°F)	5 seconds	40
	60°C(140°F)	40 seconds	
	Collect the signals (FAM/JOE*/Cy5)		

* JOE/VIC/HEX



In the software operation interface of the Applied Biosystems 7500 real-time PCR instrument, select "ROX" from the Passive Reference pull-down menu.

[Interpretation of Results]

Assessment of clinical specimen test results should be performed after the positive and negative controls have been examined and determined to be valid. If the controls are not valid, the patient results cannot be interpreted.

Open the experiment data with the analysis software and perform the Ct analysis according to the instrument manual. See the table below for the Ct cut-off for each fluorescent channel.

STANDARD M nCoV Real-Time Detection kit

Target	Ct Value	Interpretation
ORF1ab gene (FAM)	Ct≤36	SARS-CoV-2 ORF1ab (RdRp) gene positive
E gene (JOE/VIC/HEX)	Ct≤36	Coronavirus E gene positive
IC (CY5)	Ct≤26	Internal control positive

Refer to the table below for the validity and the interpretation of each specimen result according to the results of each channel.

ORF1ab(RdRp) gene (FAM)	E gene (JOE/VIC/HEX)	IC (Cy5)	Interpretation	Action to be taken
Positive	Positive or Negative	Positive or Negative	• SARS-CoV-2 Positive	Report results to sender and appropriate health authority.
Negative	Positive	Positive or Negative	• SARS-CoV-2 Presumptive Positive.	Sample is repeated once. If the repeated result remains “PRESUMPTIVE POSITIVE”, additional confirmatory testing may be conducted, if it is necessary to differentiate between SARS-CoV-2 and other SARS-like viruses for epidemiological purposes or clinical management.
Negative	Negative	Positive	• SARS-CoV-2 Negative	Report results to sender
Negative	Negative	Negative	• Invalid	Sample is repeated once from extraction. If a second failure occurs, it is reported to sender as invalid and recommend recollection if patient is still clinically indicated.



If the target gene signal (FAM, JOE/VIC/HEX) is strong, the CY5 (IC) may be negative.

13. Quality Control

All test controls should be examined prior to interpretation of patient results. If the controls are not valid, the patient results cannot be interpreted. A negative control and a positive control should be set for each batch.

The internal control A is a pseudovirus that contains RNA target, detected by the IC primers/probe set in the STANDARD M nCoV Real-Time Detection kit. Internal control A can be added to patient specimens, prior to extraction, to serve as a total process control OR can be added directly to the RT-PCR master mix, to serve as a reverse transcription and PCR amplification only control (see section 12.1 for preparation details). The internal control A should also be added to the positive control tube and negative control tube to confirm PCR amplification in each tube. Check the instrument, reagents and amplification conditions for errors and repeat the experiment.

Control	QC requirements		
	ORF1ab(RdRp) gene (FAM)	E gene (JOE/VIC/HEX)	IC (Cy5)
2019-nCoV Positive control	Ct≤26	Ct≤26	Ct≤26
Negative control	Ct>36.	Ct>36.	Ct≤26
Extraction control* (Internal control A)	-	-	Ct≤26

* If IC is only used without specimen as extraction control, Ct value of ORF1ab(RdRp) gene and E gene do not appear.

14. Limitations of the Kit Protocols

The use of this assay as an *in vitro* diagnostic under the FDA Emergency Use Authorization (EUA) is limited to laboratories that are certified under the Clinical Laboratory Improvement Amendments of 1988 (CLIA), 42 U.S.C. § 263a, to perform high complexity tests.

Use of this assay is limited to personnel who are trained in the procedure. Failure to follow these instructions may result in erroneous results.

Specimens must be collected, transported, and stored using appropriate procedures and conditions. Improper collection, transport, or storage of specimens may hinder the ability of the assay to detect the target sequences.

Extraction and amplification of nucleic acid from clinical specimens must be performed according the specified methods listed in this procedure. Other extraction approaches and processing systems have not been evaluated.

False-negative results may arise from:

- o Improper specimen collection
- o Degradation of the viral RNA during shipping/storage
- o Using unauthorized extraction or assay reagents
- o The presence of RT-PCR inhibitors
- o Mutation in the SARS-CoV-2 virus
- o Failure to follow instructions for use

False-positive results may arise from:

- o Cross contamination during specimen handling or preparation
- o Cross contamination between patient samples
- o Specimen mix-up
- o RNA contamination during product handling

The effect of vaccines, antiviral therapeutics, antibiotics, chemotherapeutic or immunosuppressant drugs have not been evaluated.

Negative results do not preclude infection with SARS-CoV-2 virus and should not be the sole basis of a patient management decision.

A positive result indicates the detection of nucleic acid from SARS-CoV-2.

Nucleic acid may persist even after the virus is no longer viable.

Laboratories are required to report all positive results to the appropriate public health authorities.

Testing of nasal, oropharyngeal, and mid-turbinate nasal swabs (self-collected on site or collected by a healthcare provider) is limited to patients with symptoms of COVID-19. Please refer to FDA's FAQs on Diagnostic Testing for SARS-CoV-2 for additional information.

Based on the in silico analysis, SARS-CoV may cross-react with the STANDARD M nCoV Real-Time Detection kit. SARS-CoV is not known to be currently circulating in the human population, therefore is highly unlikely to be present in patient specimens.

15. Conditions of Authorization

The STANDARD M nCoV Real-Time Detection kit assay's Letter of Authorization¹, User Manual, and Labeling are available on FDA website: <https://www.fda.gov/medical-devices/emergency-situations-medical-devices/emergency-use-authorizations#covid19ivd>.

To assist clinical laboratories using the STANDARD M nCoV Real-Time Detection kit, the relevant Conditions of Authorization are listed below.

- a) Authorized laboratories using your product will include results and reports of your product. Under exigent circumstances, other appropriate methods for disseminating may be used, which may include mass media.
- b) Authorized laboratories using your product will use your product as outlined in the Instructions for Use only. Deviation from the authorized procedures, such as the authorized instruments, authorized extraction methods, authorized clinical specimen types, authorized control materials, authorized other ancillary reagents and authorized materials required to use your product are not permitted.
- c) Authorized laboratories that receive your product will notify the relevant public health authorities of their intent to run your product prior to initiating testing.
- d) Authorized laboratories using your product will have a process in place for reporting test results to healthcare providers and relevant public health authorities.
- e) Authorized laboratories will collect information on the performance of your product and report to DMD/OHT7-OIR/OPEQ/CDRH (via email: CDRH-EUA-Reporting@fda.hhs.gov) and SD Biosensor (via email: sales@sdbiosensor.com) if they become aware of any suspected occurrence of false positive or false negative results and significant deviations from the established performance characteristics of your product.
- f) All laboratory personnel using your product must be appropriately trained in RT-PCR techniques and use appropriate laboratory and personal protective equipment when handling this kit and use your product in accordance with the authorized labeling.
- g) SD Biosensor, authorized distributors, and authorized laboratories using your product will ensure that any records associated with this EUA are maintained until otherwise notified by FDA. Such records will be made available to FDA for inspection upon request.

¹ The letter of authorization refers to, "Laboratories certified under the Clinical Laboratory Improvement Amendments of 1988 (CLIA), 42 U.S.C. §263a, to perform high complexity tests" as "authorized laboratories."

16. Non-clinical Performance Evaluation

16.1 Analytical Sensitivity - Limit of Detection (LoD)

The LoD study established the lowest concentration of SARS-CoV-2 (genome copies(cp)/ μ L) that can be detected by the STANDARD M nCoV Real-Time Detection kit at least 95% of the time. The LoD was established by testing twenty replicates of six different dilutions of SARS-CoV-2 viral genomic RNA spiked into both sputum and nasopharyngeal swab specimen (collected in UTM). The study results that are summarized in the tables below show that the LoD for the STANDARD M nCoV Real-Time Detection kit is 0.5 cp/ μ L for upper and lower respiratory specimens on the ABI 7500; 0.25 cp/ μ L for upper respiratory specimens and 0.125 cp/ μ L for lower respiratory specimens on the CFX95; and 0.5 cp/ μ L for upper respiratory specimens and 0.25 cp/ μ L for lower respiratory specimens on the LC480

Table 1. Results of the Analytical Sensitivity for the STANDARD M nCoV Real-Time Detection kit on the ABI 7500

Specimen type	Concentration (cp/ μ L)	ORF1ab (RdRp) gene Target			E gene Target		
		Positive replicates	Mean Ct value	Standard Deviation	Positive replicates	Mean Ct value	Standard Deviation
NP swabs	1	20/20	33.1	0.6	20/20	32.4	0.7
	0.5	20/20	33.7	0.7	20/20	34.0	0.8
	0.25	17/20	35.3	0.9	16/20	35.1	0.7
	0.125	10/20	35.3	0.6	12/20	35.4	0.8
	0.0625	9/20	35.6	0.4	9/20	36.0	0.4
	0.0312	2/20	35.5	0.7	2/20	36.5	0.6
Sputum	1	20/20	31.6	0.3	20/20	32.1	0.7
	0.5	20/20	31.5	0.3	20/20	31.2	0.3
	0.25	18/20	32.9	0.4	19/20	32.8	0.4
	0.125	13/20	34.1	0.8	18/20	33.8	0.6
	0.0625	8/20	35.2	0.6	13/20	35.0	0.8
	0.0312	3/20	35.6	0.4	11/20	35.6	0.6

Table 2. Results of the Analytical Sensitivity for the STANDARD M nCoV Real-Time Detection kit on the CFX96

Specimen type	Concentration (cp/ μ L)	ORF1ab (RdRp) gene Target			E gene Target		
		Positive replicates	Mean Ct value	Standard Deviation	Positive replicates	Mean Ct value	Standard Deviation
NP swabs	1	20/20	30.9	0.1	20/20	31.2	0.2
	0.5	20/20	32.2	0.3	20/20	32.3	0.3
	0.25	20/20	33.2	0.4	19/20	33.1	0.5
	0.125	18/20	34.3	0.8	18/20	34.1	0.6
	0.0625	16/20	34.5	0.7	15/20	34.9	0.7
	0.0312	11/20	35.3	0.8	8/20	35.8	0.5
Sputum	1	20/20	31.1	0.4	20/20	31.3	0.3
	0.5	20/20	32.1	0.3	20/20	31.9	0.4
	0.25	20/20	33.0	0.5	20/20	32.8	0.4
	0.125	19/20	34.4	0.6	17/20	34.3	0.9
	0.0625	14/20	35.3	0.5	16/20	35.0	0.5
	0.0312	10/20	35.6	0.6	12/20	35.8	0.6

Table 3. Results of the Analytical Sensitivity for the STANDARD M nCoV Real-Time Detection kit on the LC480

Specimen type	Concentration (cp/uL)	ORF1ab (RdRp) gene Target			E gene Target		
		Positive replicates	Mean Ct value	Standard Deviation	Positive replicates	Mean Ct value	Standard Deviation
NP swabs	1	20/20	31.6	0.5	20/20	32.4	0.7
	0.5	20/20	32.6	0.3	20/20	33.0	0.6
	0.25	18/20	34.8	1.1	17/20	35.2	0.8
	0.125	14/20	36.2	0.6	10/20	36.0	0.7
	0.0625	9/20	36.5	0.7	6/20	37.01	0.5
	0.0312	4/20	37.6	0.8	1/20	38.3	NA
Sputum	1	20/20	31.1	0.5	20/20	31.3	0.4
	0.5	20/20	31.0	0.2	20/20	31.3	0.3
	0.25	20/20	31.9	0.4	20/20	32.2	0.5
	0.125	17/20	33.0	0.9	16/20	33.5	0.6
	0.0625	12/20	35.1	0.5	15/20	35.1	0.6
	0.0312	7/20	35.0	1.1	11/20	35.5	0.7

16.2 Analytical Sensitivity - Reactivity/Inclusivity

In silico analysis conducted to the primers and probe showed that STANDARD M nCoV Real-Time Detection kit will detect all SARS-CoV-2 sequences in NCBI and GISAID databases. The sequences of *in silico* analysis is the full genome sequences of SARS-CoV-2 except partial sequence and miss reading sequence

Table 4. Results of *In Silico* analysis of ORF1ab(RdRp) primer/probe set

No. of Sequence ID analyzed	NCBI =1,084 and GISAID = 10,198
No. of Sequence ID of 100% Homology	11,279
No. of Sequence ID of less than 100% Homology	3

The STANDARD M nCoV Real-Time Detection kit showed 100% homology to 11,279 out of 11,282 sequences against the ORF 1ab(RdRP) primers and probe set. The 3 mismatched sequences were confirmed to single nucleotide mismatch each.

Table 5. Results of *In Silico* analysis of E primer/probe set

No. of Sequence ID analyzed	NCBI =1,084 and GISAID = 10,198
No. of Sequence ID of 100% Homology	11,278
No. of Sequence ID of less than 100% Homology	4

STANDARD M nCoV Real-Time Detection kit showed 100% homology to 11,278 out of 11,282 sequences against the E primers and probe set. The 4 mismatched sequences were confirmed to single nucleotide mismatch each.

16.3 Analytical Specificity:

a) Cross-Reactivity: Cross-reactivity of the STANDARD M nCoV Real-Time Detection kit was evaluated both *in silico* analysis and by wet-testing whole organisms/viruses purchased from ATCC.

a-1) *In Silico* analysis

In silico analysis of the primers and probes was performed against the organisms and viruses listed in Table 6. According to In-silico analysis of E primers and probe, the cross reactivity except SARS-coronavirus and other Sarbecovirus is not expected.

Table 6. Organisms and viruses evaluated for cross-reactivity, by *in silico* analysis, against the primers and probes for SARS-CoV-2 from the STANDARD M nCoV Real-Time Detection kit.

Organism
Human coronavirus OC43
Human coronavirus HKU1
Human coronavirus 229E
Human coronavirus NL63
SARS-coronavirus
MERS-coronavirus
Parainfluenza virus 1
Parainfluenza virus 2
Parainfluenza virus 3
Parainfluenza virus 4
Enterovirus(EV68)
<i>Mycobacterium tuberculosis</i>
<i>Bordetella pertussis</i>
<i>Pneumocystis jirovecii</i>
Influenza C
Parechovirus
<i>Corynebacterium diphtheriae</i>
<i>Neisseria elongata</i>
<i>Neisseria meningitidis</i>
<i>Pseudomonas aeruginosa</i>
<i>Staphylococcus epidermis</i>
<i>Streptococcus salivarius</i>
<i>Leptospira interrogans</i>
<i>Chlamydia psittaci</i>
<i>Coxiella burneti</i> (Q-Fever)

a-2) Cross-reactivity Wet Tested

The 22 organisms and viruses, listed in Table 7, were wet-tested for cross-reactivity with the STANDARD M nCoV Real-Time Detection kit. All organisms and viruses were tested by spiking the organism/virus into NP swab matrix mixed with lysis buffer at the concentrations listed in Table 7. Each organism/virus was tested for cross-reactivity, in triplicate, on the CFX96. No cross-reactivity was observed for the organisms and viruses listed Table 7.

Table 7. Cross-reactivity Test

No.	Category	Cross-reactivity substance	Specimen Info.	Spiking Concentration
1	Non 2019-nCoV coronavirus infections	MERS-CoV	ATCC VR-3248SD	1 x 10 ⁵ copy/ml
		HCoV-229E	ATCC VR-740	1 x 10 ⁶ PFU/mL
		HCoV-HKU1	ATCC VR-3262SD	
		HCoV-NL63	ATCC VT-3263SD	

STANDARD M nCoV Real-Time Detection kit

		HCoV-OC43	ATCC VR-1558	
2	Non 2019-nCoV Viral infections	Influenza A virus	ATCC VR-1811	
		Influenza B virus	ATCC VR-1735	
		Respiratory syncytial virus	ATCC VR-1540	
		Rhinovirus	ATCC VR-284	
		Parainfluenza virus	ATCC VR-94	
		Adenovirus	ATCC VR-3	
3	Bacteria	<i>Legionella pneumophila</i>	ATCC 33152	1 x 10 ⁶ CFU/mL
		<i>Chlamydia pneumoniae</i>	ATCC VR-2282	
		<i>Mycoplasma pneumoniae</i>	ATCC 15531	
		<i>Haemophilus influenzae</i>	ATCC 10211	
		<i>Moraxella catarrhalis</i>	ATCC 25240	
		<i>Streptococcus pyogenes</i>	ATCC 19615	
		Bowman Animal bacterium	ATCC 19606	
		<i>Klebsiella pneumoniae</i>	ATCC 13883	
		<i>Pseudomonas aeruginosa</i>	ATCC 27853	
<i>Streptococcus pneumonia</i>	ATCC 6301			
4	Pooled human nasal wash		Employee	5-50%

17. Clinical Performance Evaluation

The performance of the STANDARD M nCoV Real-Time Detection kit was evaluated in a contrived clinical study using 30 nasopharyngeal specimens (NP) (collected in UTM) and 30 sputum samples collected from patients with signs and symptoms of a respiratory infection. Each specimen was split in order to prepare 30 positive and 30 negative samples for clinical evaluation. Positive samples were prepared by spiking viral genomic RNA at 2X and 4X LoD into 30 NP samples and 30 sputum samples, premixed with lysis buffer. All samples were extracted using the QIAamp Viral RNA Mini kit and were measured on the ABI 7500. All samples were tested in randomized and blinded fashion. The positive and negative percent agreements between the STANDARD M nCoV Real-Time Detection kit and the expected results from the NP swab and sputum specimens are shown below:

Table 8. Result of clinical study

Specimen type	Sample Concentration	N	ORF1ab_RdRp gene		E gene	
			% positive	Mean Ct	% positive	Mean Ct
Nasopharyngeal swab specimen(UTM)	2x LOD	20	100	32.22	100	31.84
	4x LOD	10	100	30.80	100	30.93
	Negative	30	0	-	0	-
Sputum	2x LOD	20	100	31.92	100	31.32
	4x LOD	10	100	31.10	100	30.50
	Negative	30	0	-	0	-

All positive samples were positive and all negative samples were negative in the background of individual clinical sample matrix.

In conclusion, the performance against the expected results are:

Table 9. Result of clinical study

Specimen	Result
Nasopharyngeal swab specimen(UTM)	<ul style="list-style-type: none"> • Positive Percent Agreement: 100%(30/30) [95% CI: 88.65 – 100%] • Negative Percent Agreement: 100%(30/30) [95% CI: 88.65 – 100%]
Sputum	<ul style="list-style-type: none"> • Positive Percent Agreement: 100%(30/30) [95% CI: 88.65 – 100%] • Negative Percent Agreement: 100%(30/30) [95% CI: 88.65 – 100%]

18. Troubleshooting

1. If the PC and IC are invalid: check for the expiration date indicated on the box label due to the possibility of invalidity of the expiration date or for improper storage conditions.
2. If the IC is invalid: check the results of the other tubes to see if they have been added to the PCR mixture. If the target Ct is ≤ 25 Ct, the IC may not be detected due to the overflow of the target amplicon.
3. If NC is invalid: this may be due to contamination of the workplace or the equipment, or improper storage.

19. Reference

1. Clinical management of severe acute respiratory infection when novel coronavirus (nCoV) infection is suspected. Interim guidance. WHO.2020
2. Diagnostic detection of Wuhan coronavirus 2019 by real-time RT-PCR.2020
3. Diagnosis and treatment of pneumonia caused by new coronavirus (trial version 4) National Health Commission. 2020
4. CDC Interim Guidelines for Collecting, Handling, and Testing Clinical Specimens from Persons Under Investigation (PUIs) for Coronavirus Disease 2019 (COVID-19)
<https://www.cdc.gov/coronavirus/2019-nCoV/lab/guidelines-clinical-specimens.html>