


Manufacturing and Distributing Respirators for Health Care Use in the United States Under an Existing Emergency Use Authorization (EUA) During the COVID-19 Pandemic

- To distribute respirators for health care use in the United States, the respirators must be FDA cleared or be authorized under an [FDA EUA](#).
- For information about the NIOSH Respirator Approval Program, consider the information provided by NIOSH NPPTL* at: <https://www.cdc.gov/niosh/npptl/RespApprovalInfo.html>
- If you are manufacturing outside the United States, see [Information for Filing Personal Protective Equipment and Medical Devices During COVID-19](#)

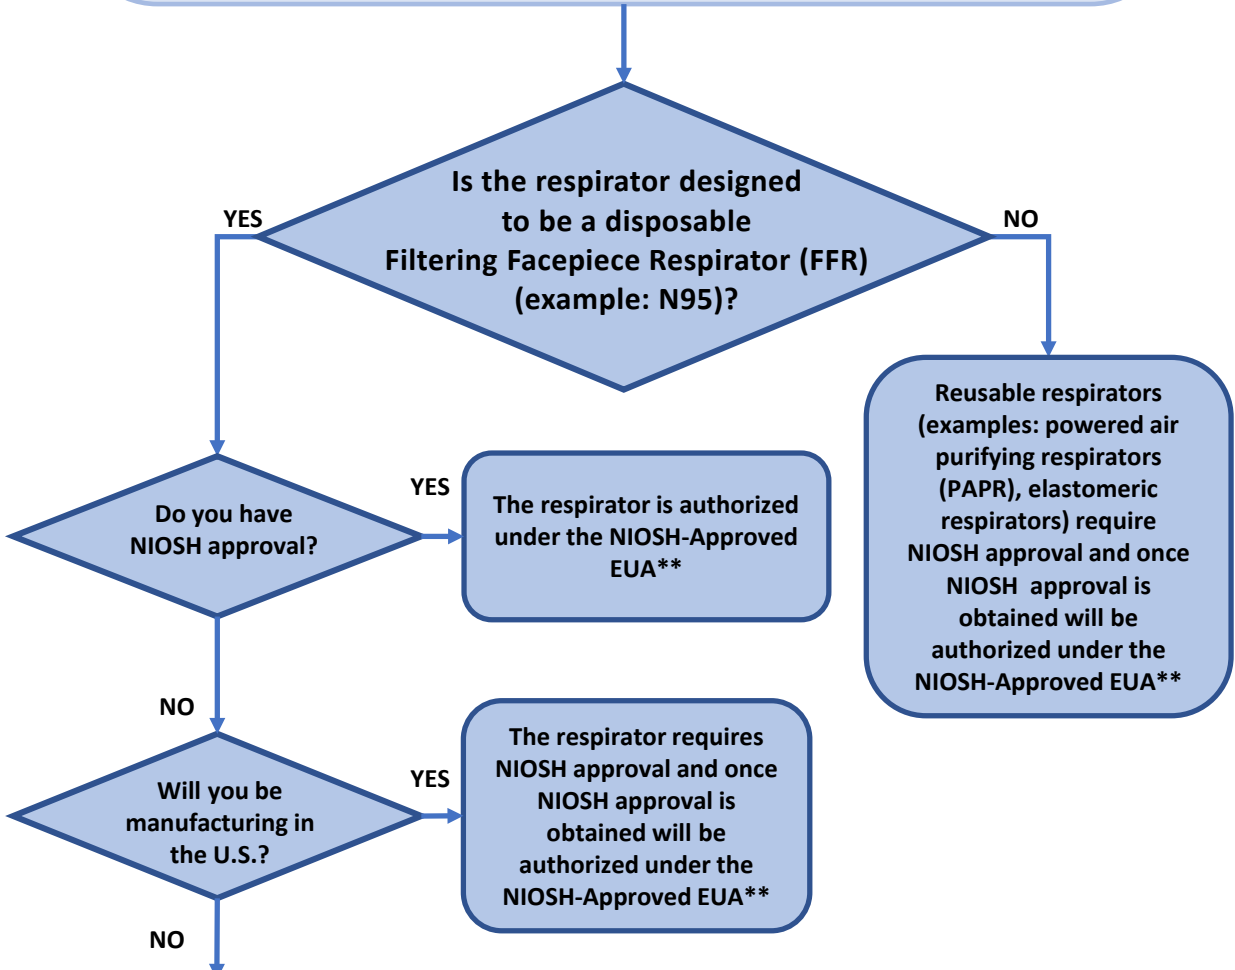

If manufactured in China, requires FDA clearance or authorization under the [Non-NIOSH-Approved EUA for China#](#)

If manufactured elsewhere, requires FDA clearance or authorization under the [Non-NIOSH-Approved EUA##](#)

*NIOSH (National Institute for Occupational Safety and Health (NIOSH) National Personal Protective Technology Laboratory (NPPTL)

**[NIOSH-Approved EUA](#) refers to the FDA EUA for NIOSH-Approved Air-Purifying Respirators

[#Non-NIOSH-Approved EUA for China](#) refers to the FDA EUA for Non-NIOSH-Approved Disposable Filtering Facepiece Respirators Manufactured in China

[##Non-NIOSH-Approved EUA](#) refers to the FDA EUA for Non-NIOSH-Approved Disposable Filtering Facepiece Respirators