

# How to collect a nasal swab sample




Read instructions entirely. Failure to follow the instructions entirely may lead to false or incomplete results. Only collect the sample on the day you are scheduled to drop it off and only drop off your own sample.




## 1 Blow your nose.

Thoroughly blow and wipe your nose to clear thick mucus (snot).




## 2 Wash your hands.

Wash with soap and water for at least 20 seconds or use hand sanitizer and dry completely.




## 3 Open the package with the swab.

**Careful: Don't touch the soft tip with your hands.** Peel open where indicated. Leave swab in the package for now.



## 4 Pull up to remove the cap from the collection tube.

Place it on a clean surface where you can easily find it.




## 5 Pick up the swab.

Pull swab out of its packaging, **being careful not to touch the soft tip with your hands.** Have the tube ready to put the swab in after collecting the sample.




## 6 Collect sample from nostril.

Insert the swab into one nostril **just until the soft tip is no longer visible.** Rotate it in a circle around the inside edge of your nostril 3 times.




## 7 Collect sample from other nostril.

Use the same soft tip to repeat the previous step in the second nostril 3 times.




## 8 Put the swab in the collection tube.

The soft tip of the swab that went into your nose should go into the tube first.




## 9 Push cap down firmly.

Push the cap straight down onto the tube until it cannot go down any farther.




## 10 Wash your hands.

Wash with soap and water for at least 20 seconds or use hand sanitizer and dry completely.



## 11 Put the tube into the sealable bag.

Seal the bag and write your name on it.



## 12 Deliver to collection site *today*.


See instructions on the reverse side.

Questions? Call support line at (617) 714-7590 or e-mail [crsp-careevolve@broadinstitute.org](mailto:crsp-careevolve@broadinstitute.org)


This self-collection kit has not been FDA cleared or approved. The test used with this kit has been authorized by FDA under an EUA for use by the authorized laboratory. This self-collection kit has been authorized only for the detection of nucleic acid from SARS-CoV-2, not for any other viruses or pathogens. This self-collection kit is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of in vitro diagnostics for detection and/or diagnosis of COVID-19 under Section 564(b)(1) of the Federal Food, Drug, and Cosmetic Act, 21 U.S.C. § 360bbb-3(b)(1), unless the authorization is terminated or revoked sooner.




When you arrive at the drop-off location, you will provide identification.

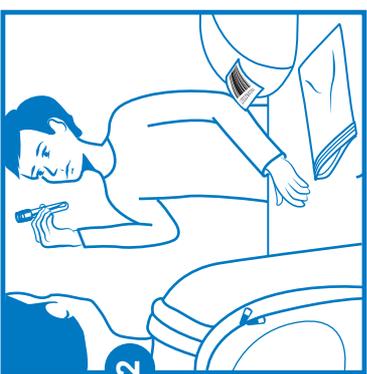

Hand the bagged sample to the drop-off technician, who will inspect it. If there is a noticeable issue, you will step aside to a re-testing station.

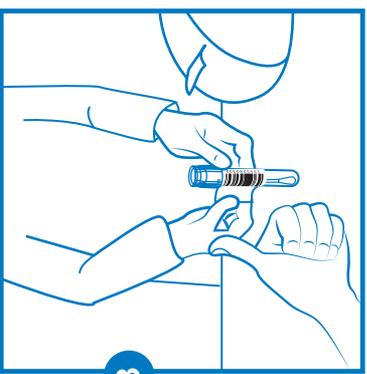

The technician will print the barcode, show it to you to confirm that the information is correct, and affix it to your tube.

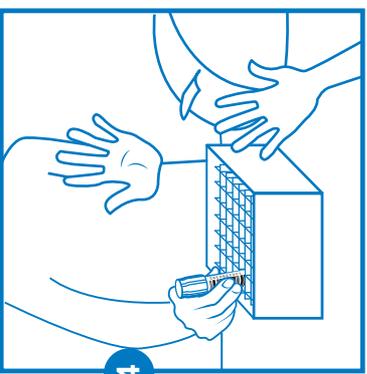


The technician will place the sample in a box rack. You are done!

# How to deliver a nasal swab sample

## Contents of testing kit

Unfold booklet and follow complete instructions.

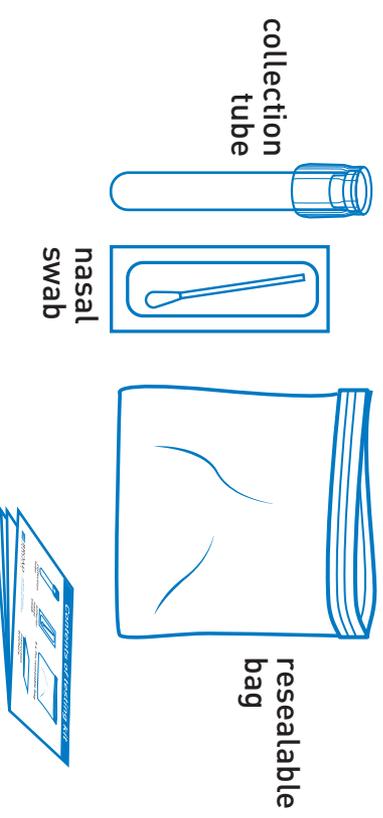

See reverse side for kit contents and open booklet for full instructions.



Read instructions entirely. Failure to follow the instructions entirely may lead to false or incomplete results.

Only collect the sample on the day you are scheduled to drop it off and only drop off your own sample.



CLINICAL RESEARCH  
SEQUENCING PLATFORM

instruction  
brochure